



Fridge-tag® 2 L


User Guide

Table of Contents

Overview	4
Purpose	4
Key Features.....	4
Important Information	5
Liability	5
Battery.....	5
Useful Life	5
Regulatory Certification	6
Display Explanations.....	7
State of Delivery / Sleep Mode	8
Placing the Fridge-Tag	10
With an Internal Sensor	10
With an External sensor.....	10
Activation Process	11
Overview	11
Device Activation	12
Setting the Calendar Format	12
Using the READ and the SET buttons.....	13
Setting the Date.....	14
Setting the Time	16
Setting Alarm Limits (if preset by factory).....	18
Connection Error (External Sensor Only).....	21
Read and Change Settings.....	23
Overview: Menu	23

Initial Menu (Read and Change Settings).....	24
Menu Access.....	24
Screen Displays During Measurement Mode.....	26
Example OK Display – During Measurement	26
Example Alarm Display – During Measurement.....	26
Alarm Trigger Function	28
Alarm Display and Confirmation Options.....	30
Confirmation Options of Currently Triggered Alarms of the Day.....	31
Cumulative Daily Time Above/Below the Limit	33
Audio Alarm (Optional Factory Setting).....	34
Reading History / Readout Mode.....	35
Option 1: Read From Device (30-Day History).....	35
Option 2: Read Alarms on the Device (Alarm Super Jump Function).....	38
Option 3: Read Data from the Files Generated by the Fridge-Tag.....	40
PDF Report Explanation.....	42
Autoscaling of Graphs in PDF.....	44
Temperature Record Duration (Optional Factory Setting)	46
Verification process	47
Explanations of Terms	49
FAQ / Glossary.....	50
Frequently Asked Questions (FAQ).....	50
Glossary of Symbols	50

Overview

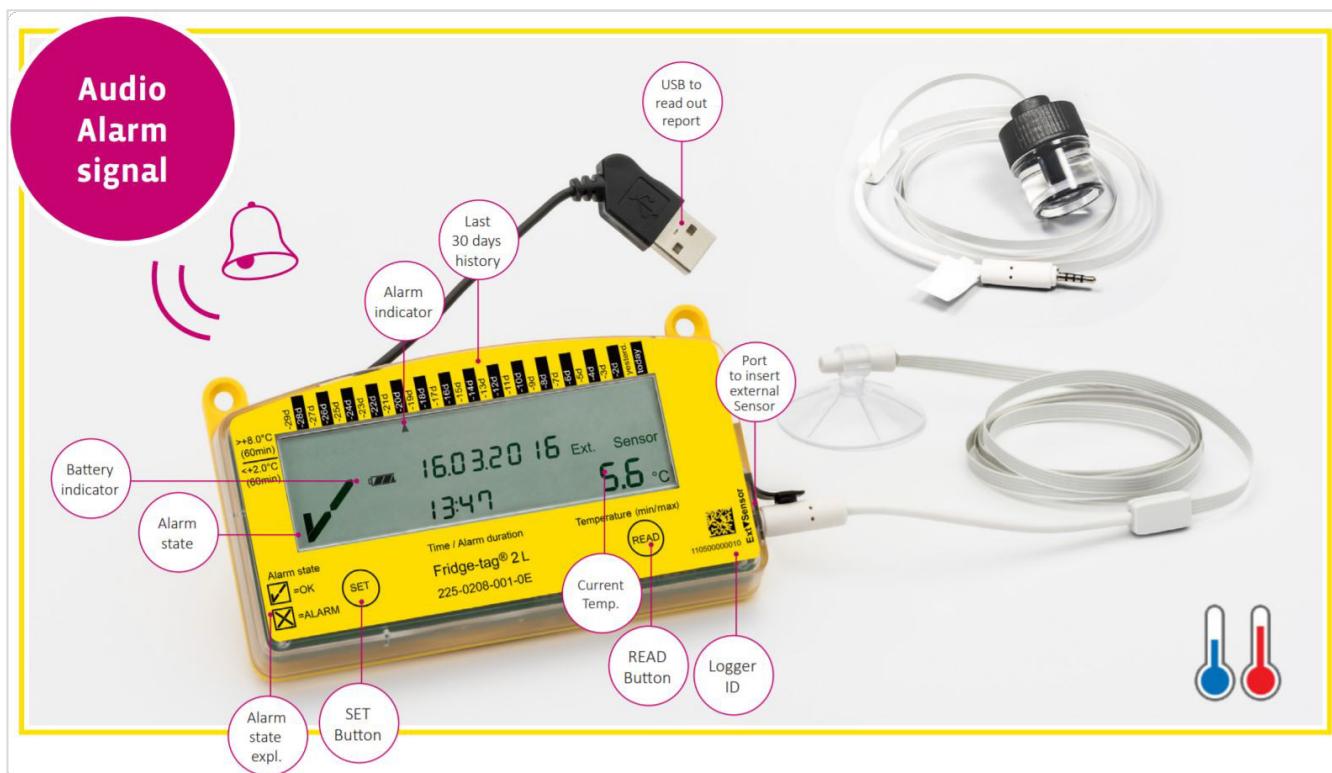

Purpose

The intended purpose of the Fridge-tag 2 L is to measure temperature in a refrigerator/freezer and create a (summary) report upon user request.

Key Features

The Fridge-tag 2 L automatically triggers an alarm, if a critical temperature deviation out of the predefined temperature range will be measured. This enables you and your staff to react just in time and avoid serious quality issues while complying with various regulations.

- **Flexible Recording Options:** Factory configurations available for 28, 56, 84, or 112 days
- **Data Verification Tools:** Software for validating PDF and ASCII files available
- **Smart Integration:** Fully compatible with Berlinger SmartView for streamlined data

Important Information

Liability

The manufacturer shall not be held liable:

- if the device was used beyond the manufacturer's given limitations.
- for any claims due to the improper storage or use of the device.
- for any problems with the temperature-controlling and/or-cooling unit.
- for the quality of any monitored goods.
- for incorrect readings if the device was used beyond its expiration date.

Battery

The Fridge-tag 2 L contains a coin cell Lithium battery. Please, pay strict attention to the following points:

- The housing of the Fridge-tag 2 L must never be opened nor destroyed.
- Never expose the Fridge-tag 2 L to high temperatures (fire, oven, microwaves, etc.). It may cause injuries.
- Always keep the Fridge-tag 2 L out of the reach of children.
- The battery complies with IATA DGR Packaging Instruction 970 Section 2.
- Dispose or recycle the Fridge-tag 2 L in accordance with the WEEE 2012/19/EU guidelines or your local regulations. The device may also be returned to the manufacturer for proper recycling.
- Remove and immediately recycle or dispose of used batteries according to local regulations and keep away from children. Do NOT dispose of batteries in household trash or incinerate.
- Call a local poison center for treatment information
- Non-rechargeable batteries are not to be recharged.
- Do not force discharge, recharge, disassemble, heat above (85° Celsius / 185 Fahrenheit) or incinerate. Doing so may result in injury due to venting, leakage or explosion resulting in chemical burns.

Useful Life

The device can be used up to 3 1/2 years after production date (1/2-year storage / 3 years useful life) on the condition that:

- Buttons are not pressed for very long time.

Note: Avoid jamming the device between the goods to be monitored in refrigerator/freezer.


- Storage and operation of the device remains inside the recommendations of the manufacturer. Especially temperatures below 0°C or +32°F could have a negative influence on the operating lifetime of the battery.

The end of the lifetime of the battery is indicated by the battery indicator on the display. Refer to the [Display Explanations](#) section).


The Fridge-tag 2 L measures the ambient temperature and not the quality of the monitored goods. Its purpose is to signal if product quality evaluation is required.

Subject to change. Please note that all information in this document is correct at the time of publication. Due to our policy of continuous product development, we reserve the right to change this information without prior notice.

Regulatory Certification

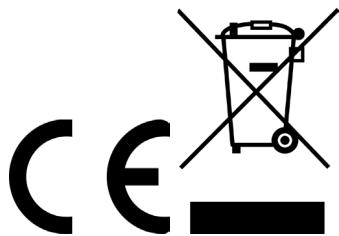

Display Explanations

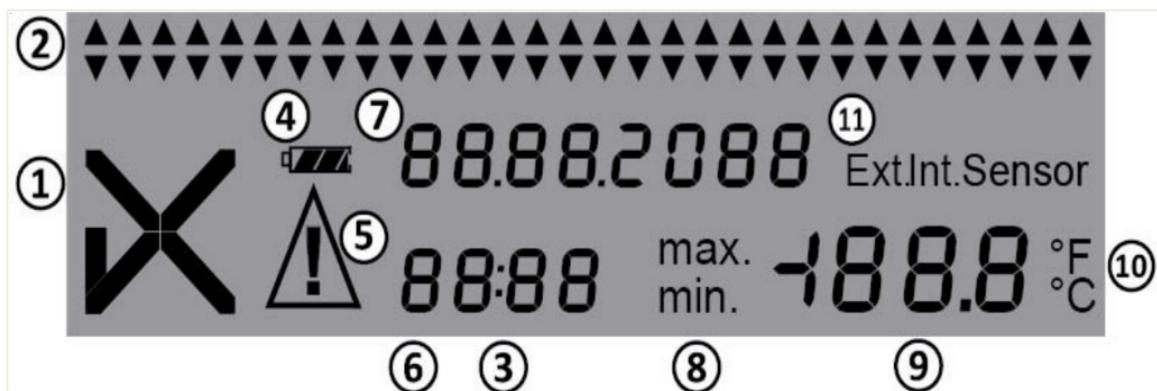


1. ✓ (OK symbol) or X (alarm symbol)
2. Daily HIGH/LOW alarm indicators ▲ ▼ (showing the history of the last 30 days)
3. Power indicator (colon is flashing)
4. Battery indicator (indicates the remaining capacity of the battery)
5. Additional warning symbol △
6. Time, duration and text display
7. Date and text display
8. Display of measured minimum/maximum temperature
9. Temperature display
10. Display of the temperature measurement unit (°F/°C)
11. Display of the activated sensor:
 - Int. = internal sensor
 - Ext. = external sensor (cable with temperature sensor)

Note: All illustrations in the User Manual refer to the Fridge-tag with internal sensor. Differences between internal and external sensors are additionally described.

State of Delivery / Sleep Mode

The Fridge-tag is shipped in sleep mode.

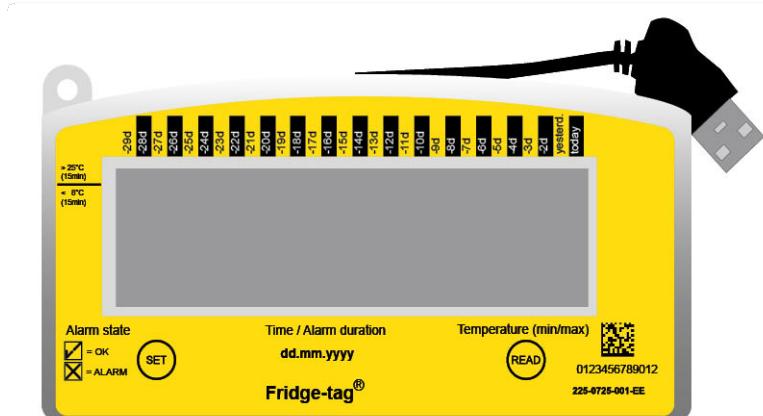

The display (LCD) is blank.


At the backside of the Fridge-tag 2 L is a backside label on which the date of activation and the location can be added.

For more information about the expiration code, please refer to the [Expire Code Explanation](#) section.

Read Out Information Prior To Activation (In Sleep Mode)

The following page shows which information will be indicated on the screen upon successive READ button pressings while in sleep mode.

Note: After approx. 60 seconds without to press any button of the Fridge-tag the devices goes back into sleep mode; the display is blank again. Start from the beginning.

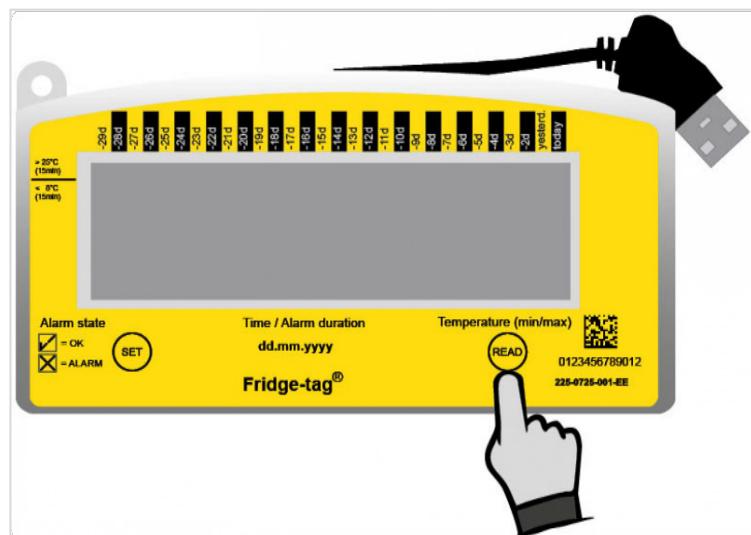

Press repeatedly READ to gather information.

After 1st pressing of READ		Display test: all segments activated
After 2nd pressing of READ		Indication of date and production test result: 16 February 2018/PASS (quality check passed)
After 3rd pressing of READ		Indication of the current temperature and which sensor is activated (internal/external). Display shows ---. --- °C if external sensor is not connected.
After 4th pressing of READ		Indication of configuration ID (e.g. 1234)
After 5th pressing of READ *		Indication of upper alarm settings. Example shows duration and temperature limits: 10 hours, >+8°C, high
After 6th pressing of		Indication of lower alarm settings. Example shows duration and temperature limits: 1 hour, <-0.5°C, low
READ *		
After 7th pressing of READ		Serial number of the device
After 8th pressing of READ		PCb number (manufacturer information)
After 9th pressing of READ		Battery power: 3 bars = full (>70%) 2 bars = half-full (>30-70%) 1 bar = low (0-30%)** **Device should be replaced.
After 10th pressing of READ		Disable user clock adjust. For more information, please see Activation Process section.
After 11th pressing of READ		The display is blank again.

*Only indicated if preset by factory, otherwise skipped.

Placing the Fridge-Tag

This section describes how to place a fridge-tag with an internal and external sensor.

With an Internal Sensor

An activated Fridge-tag must be placed immediately after activation in its predetermined location. It is recommended and important to place the device in the center of the refrigerator for an optimal temperature observation.

Please do not place the device into a freezer as the screen will freeze and the battery will lose power prematurely.

With an External sensor

Two hours before activating the Fridge-tag the external sensor must be placed in its predetermined location. It is recommended and important to place the external sensor in the center of the refrigerator for an optimal temperature observation and to avoid any incorrect measurements when starting the device.


For the right positioning of the external sensor within the fridge, please follow the instructions of WHO, CDC or any other governmental requirements of your country.



- External Sensor
- Flat cable
- Fridge-tag

Activation Process

Overview

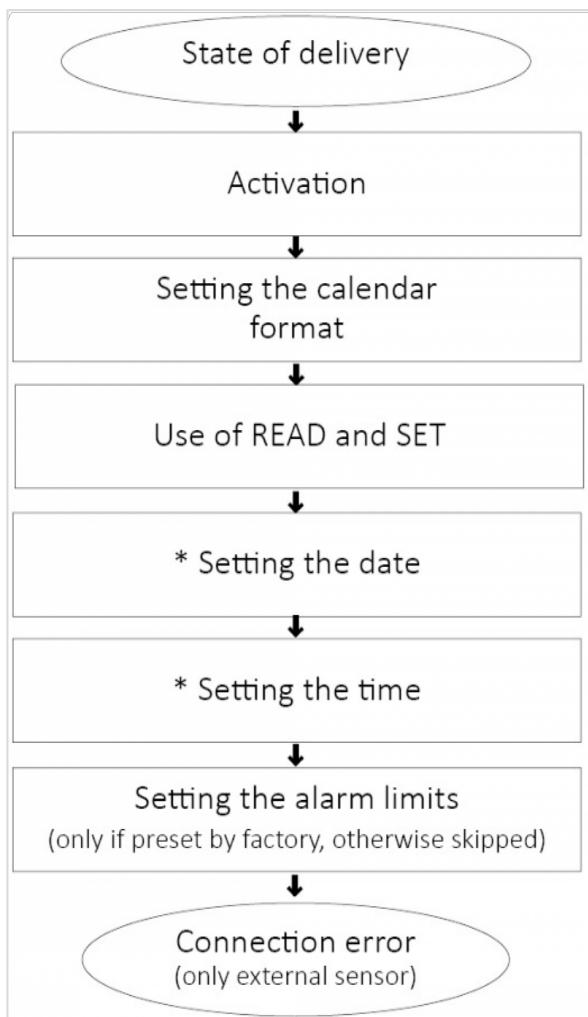


*If "Disable User Clock Adjust" in the configuration is enabled points "Setting the date" and "Setting the time" are skipped upon activation

Note: As long as the activation process has not been completed, after approx. 60 seconds without any button operation, the device will go back into sleep mode. The activation has to start from the beginning.

If you want to read or change settings (e.g. change °F to °C) after the activation has been completed, please refer to [Read and Change Settings](#).

Device Activation

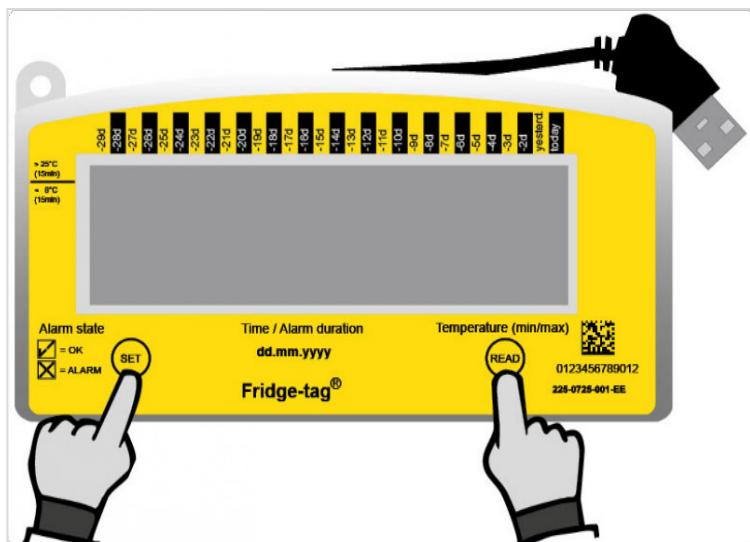

To activate the device press, the SET and the READ button simultaneously for at least 3 seconds.


Note: Once the device is activated, it cannot be stopped anymore.

Activation has been successful when the following indication appears on the screen:




Setting the Calendar Format

Option 1: DD.MM.YYYY Format

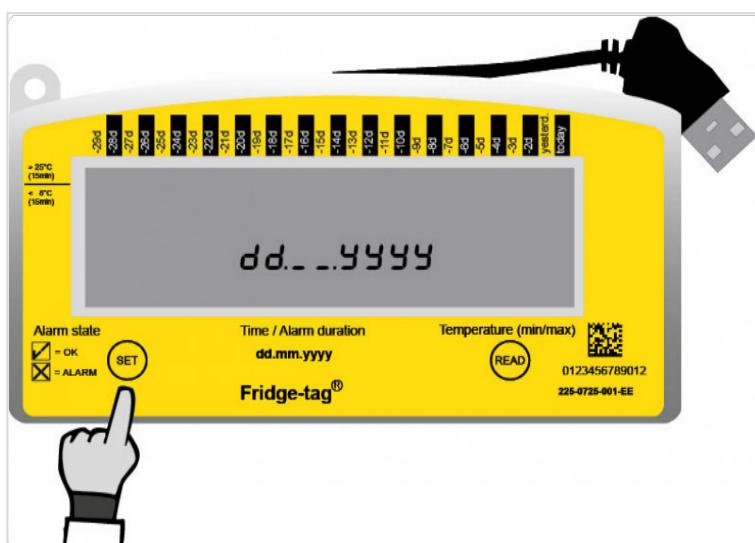

Press **SET** to save the calendar format.

Option 2: MM.DD.YYYY Format

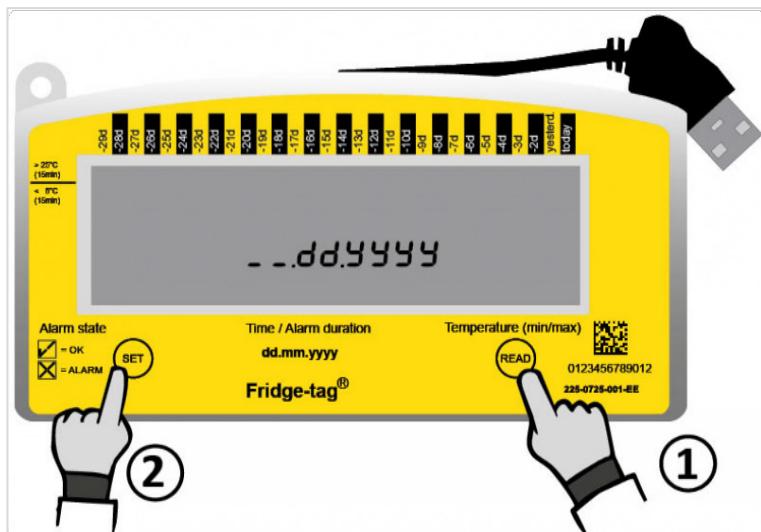


1. Press **READ** to change the calendar format.
2. Then press **SET** to save the calendar format.

After setting the calendar format, the first digit of the date will start flashing.

Using the READ and the SET buttons

READ button


The **READ** button is used to adjust the numbers. Each time you press the **READ** button, the number in the flashing digit will increase by 1. If you press **READ** more than necessary, continue pressing the **READ** button until you obtain the desired number.

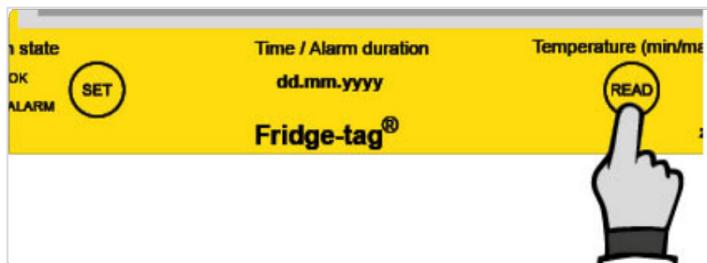

Press **READ** to adjust the number.

SET button

The **SET** button is used to save the number. After pressing the **SET** button, the next digit will start flashing.

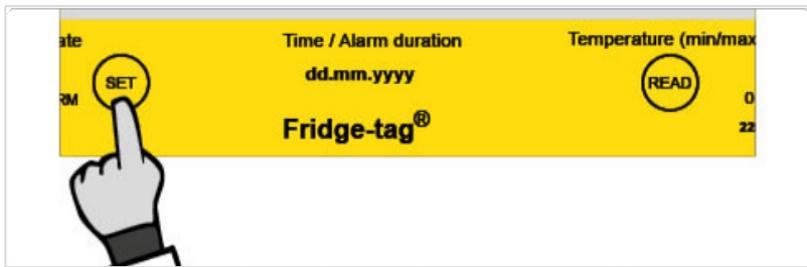

Press **SET** to confirm.


Note: If **SET** is pressed mistakenly, continue with the setup instructions.

Setting the Date

The following example shows how to set the date to: 16 February 2018 (16.02.2018) in European format.


<p>The 1st digit is flashing.</p>	<ul style="list-style-type: none"> • Press READ until "1" appears as the first digit. • Press SET to save.
<p>The 2nd digit is flashing.</p>	<ul style="list-style-type: none"> • Press READ until "6" appears as the second digit. • Press SET to save.

The 3rd digit is flashing.

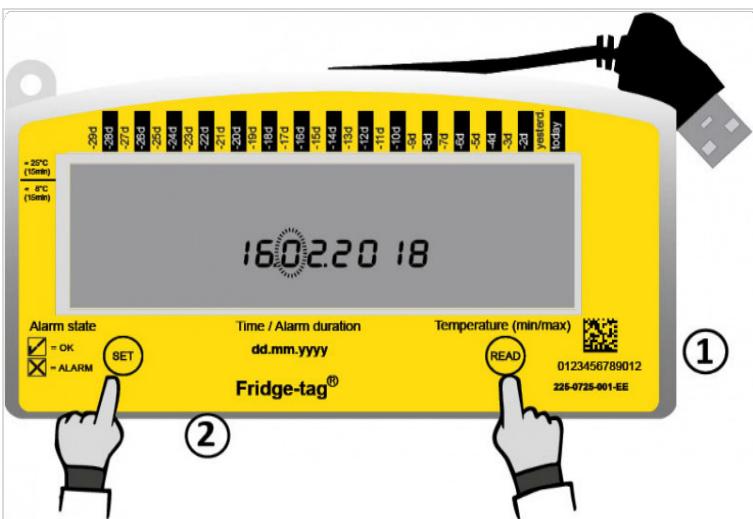

- Press **READ** until "0" appears as the third digit.
- Press **SET** to save.


The 4th digit is flashing.

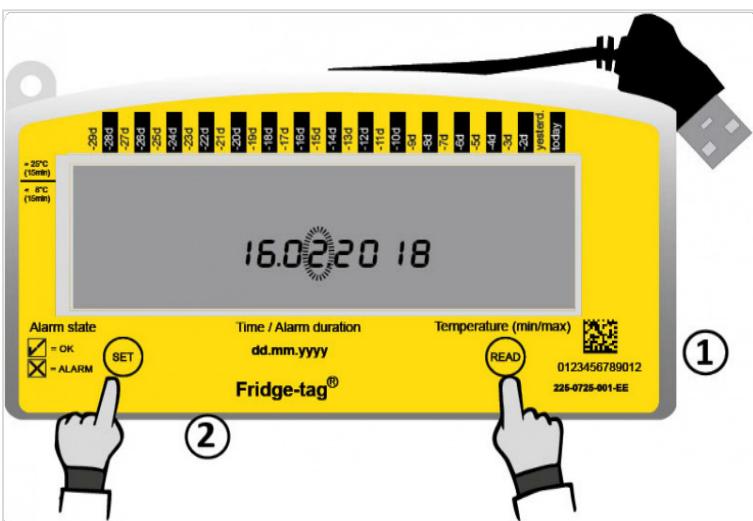

- Press **READ** until "2" appears as the fourth digit.
- Press **SET** to save.


Note: The fifth and the sixth digit are set automatically.

The 7th digit is flashing.

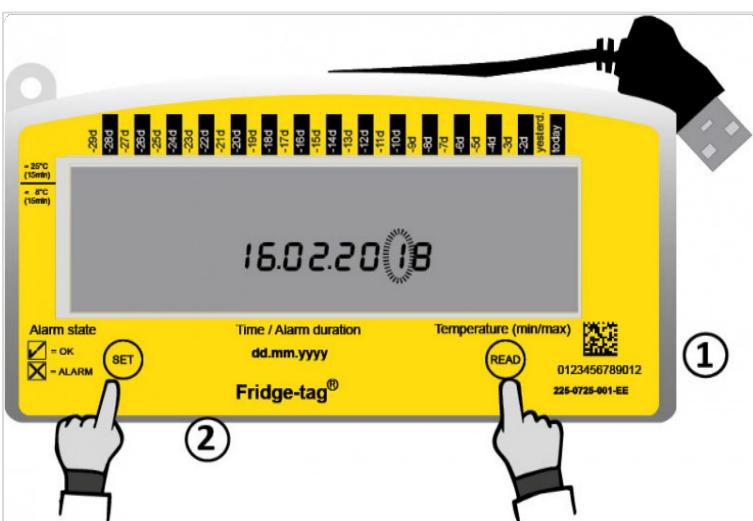

- Press **READ** until "1" appears as the seventh digit.
- Press **SET** to save.

The 8th digit is flashing.

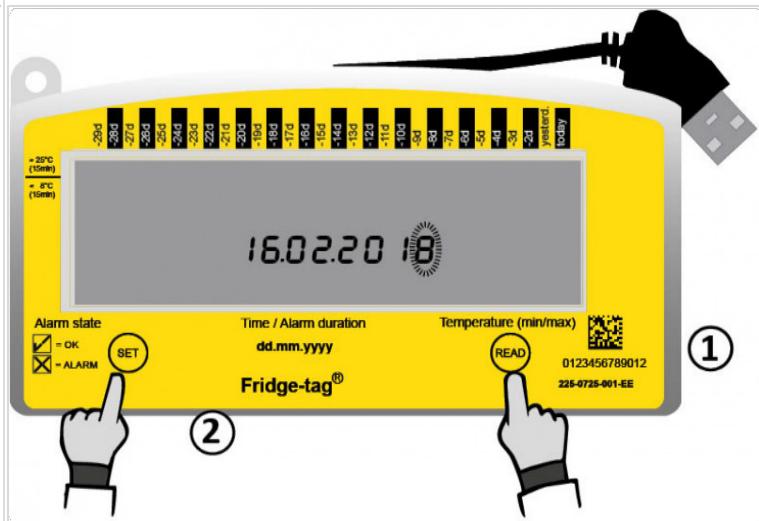

- Press **READ** until "8" appears as the eighth digit.
- Press **SET** to save.

The date is now set to: 16.02.2018.


Note: After setting the date, the first digit of the time will start flashing.

Setting the Time

This example shows how to set the time to 13:47.


Note: The clock operates a 24-hour clock (e.g. 1:47 pm = 13:47).

The 1st digit is flashing:

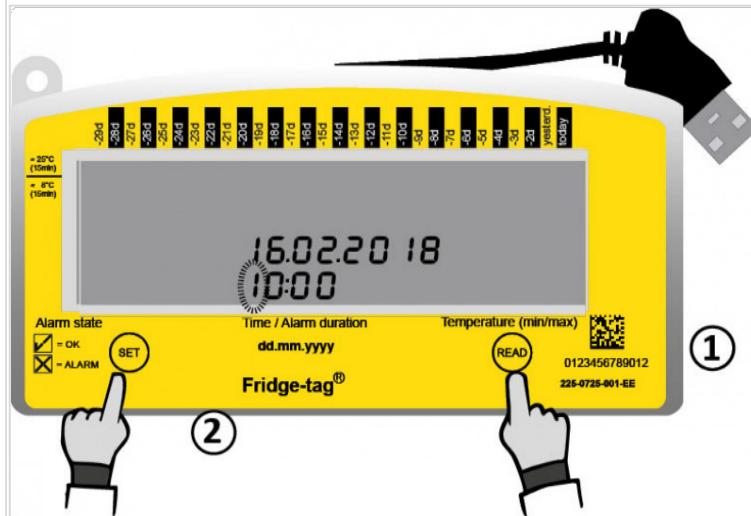


- Press **READ** until "1" appears as the first digit.
- Press **SET** to save.

The 2nd digit is flashing.

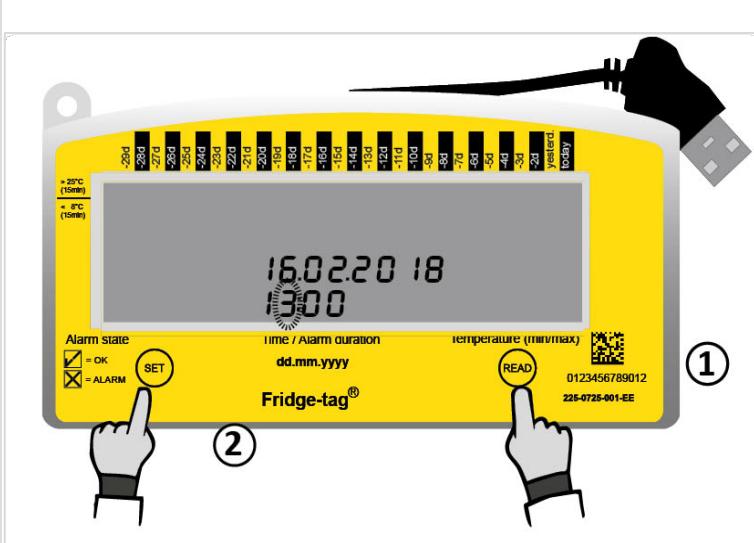


- Press **READ** until "3" appears as the second digit.
- Press **SET** to save.

The 3rd digit is flashing.

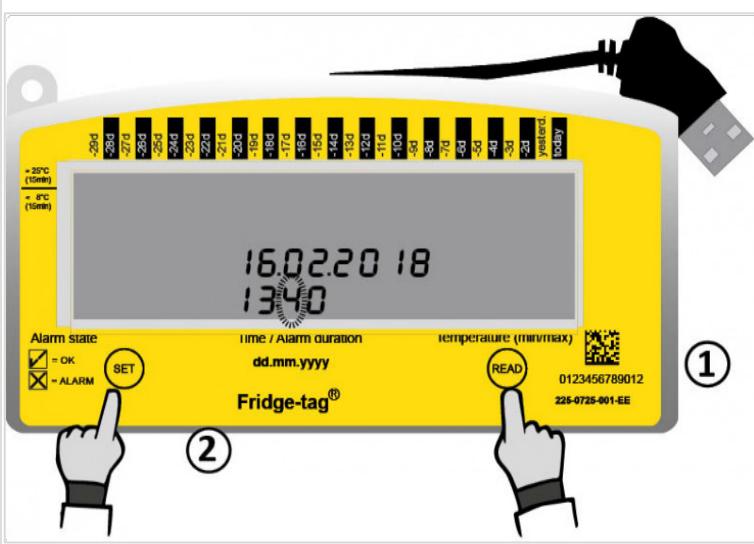

- Press **READ** until "4" appears as the third digit.
- Press **SET** to save.

The 4th digit is flashing.

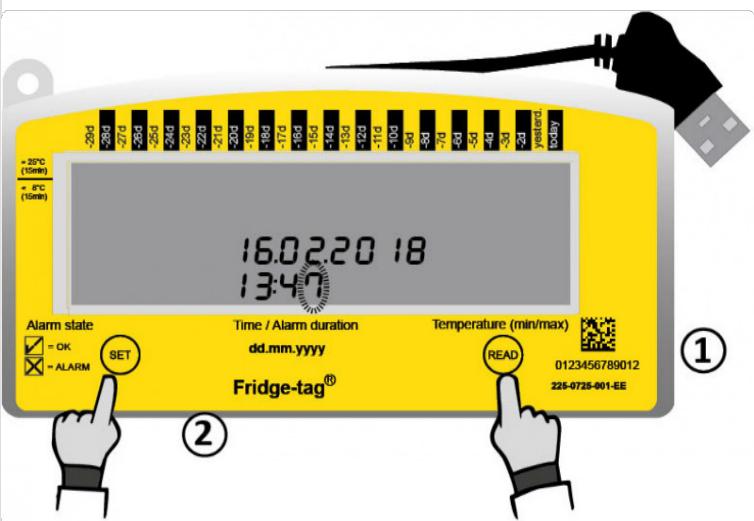

- Press **READ** until "7" appears as the fourth digit.
- Press **SET** to save.

The time is now set to 13:47.

Note: If the device is configured with self-programmable alarm limits proceed with the following [Setting Alarm Limits \(if preset by factory\)](#) section.

As soon as the last digit of the time setting is confirmed, the activation is completed.

Internal sensor: Now place the Fridge-tag. Refer to section [Placing the Fridge-Tag](#).



External sensor: Connect the device with the external sensor. During max. 1 minute after activation no temperature is displayed on the screen.

Setting Alarm Limits (if preset by factory)


This adjustment is done in 4 steps:

1. Setting the duration of the upper alarm limit
2. Setting the temperature of the upper alarm limit
3. Setting the duration to the lower alarm limit
4. Setting the temperature of the lower alarm limit

Steps 1 and 3, and steps 2 and 4 are completed in the same manner, respectively.

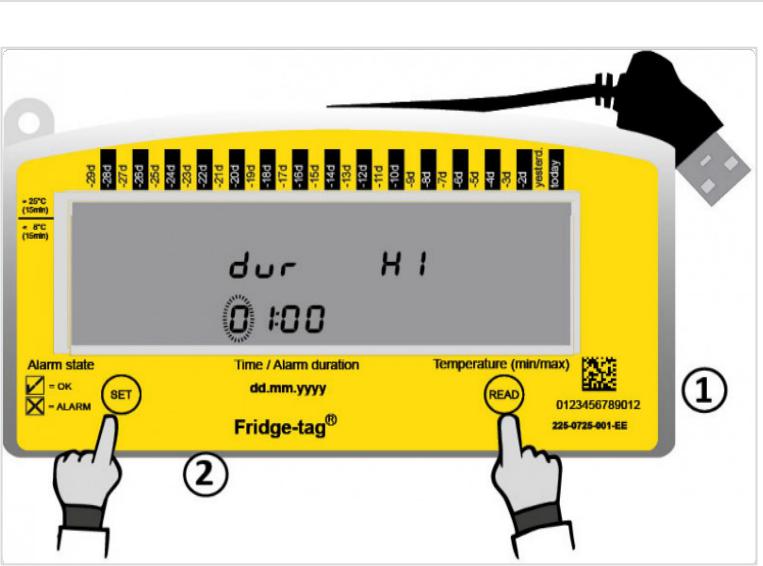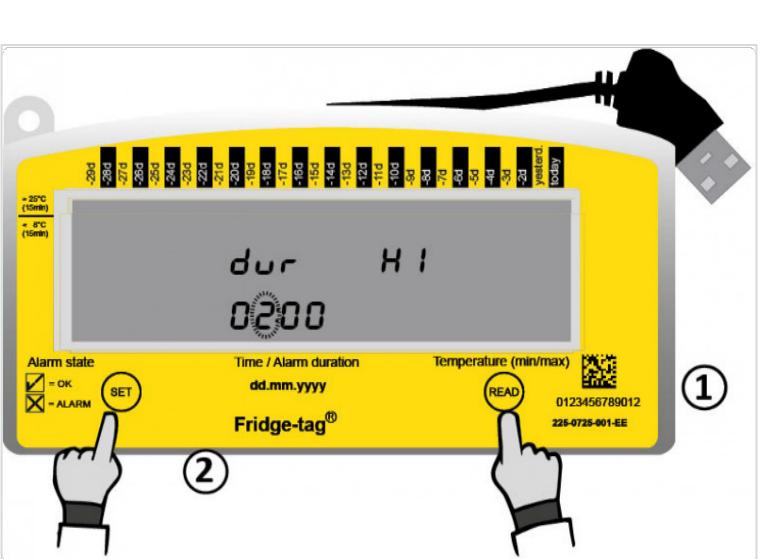
<p>The 1st digit of the duration of the alarm limit is flashing.</p> 	<ul style="list-style-type: none">• Press READ to adjust the number.• Press SET to confirm the number.
<p>The 2nd digit of the duration of the alarm limit is flashing.</p> 	<ul style="list-style-type: none">• Press READ to adjust the number.• Press SET to confirm the number.

The 3rd digit of the duration of the alarm limit is flashing.

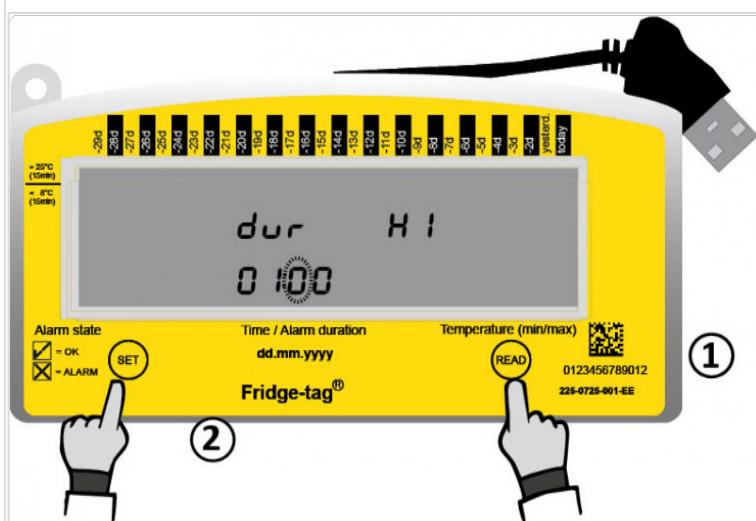

- Press **READ** to adjust the number.
- Press **SET** to confirm the number.

The 4th digit of the duration of the alarm limit is flashing.

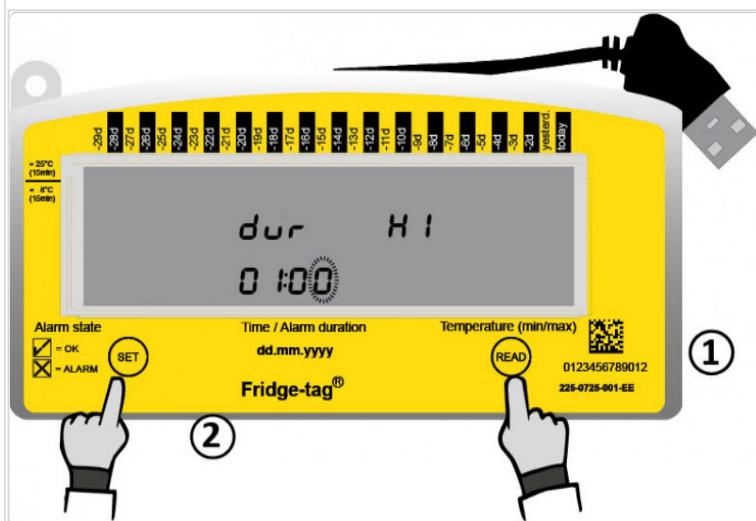

- Press **READ** to adjust the number.
- Press **SET** to confirm the number.


The duration of the alarm limit is now set.

First you have to choose the range of the desired temperature limit. You have the choice between negative and positive temperatures. In case of a positive limit in Fahrenheit you may further choose if the limit shall be equal or above +100°F. This choice is made by repeatedly pressing READ until the desired range is indicated.

- **Internal sensor:** Alarm temperature limits must be no lower than -20°C (-4°F) and no higher than +50°C (+122°F).
- **External sensor:** Alarm temperature limits must be no lower than -35°C (-31°F) and no higher than +55°C (+131°F).

Note: The temperature measurement unit (°C/°F) can only be changed after the device is activated in the menu. Refer to section [Read and Change Settings](#).

Follow the instruction for setting a positive temperature limit between 0°C/0°F and +50°C/+122°F (internal sensor) or 0°C/0°F and +55°C/+131°F (external sensor)

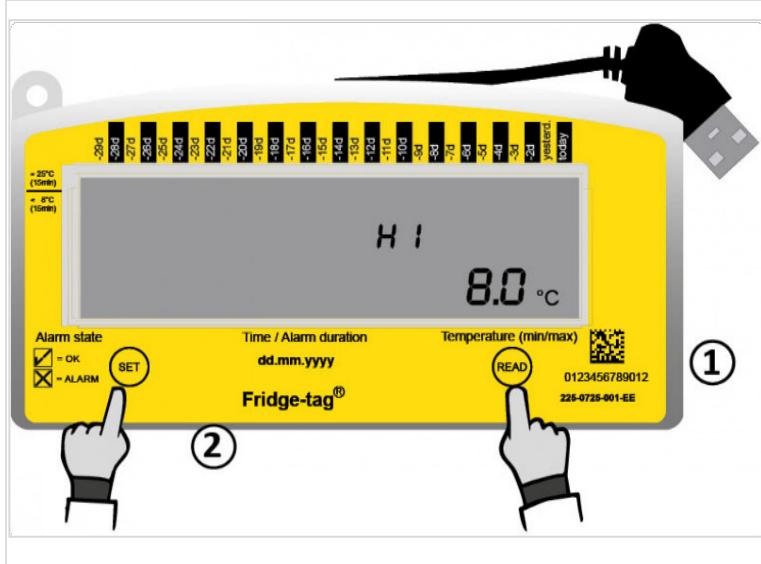


- Press **READ** until the display shows no flashing sign.
- Press **SET** to adjust the limit between 0°C/0°F and +50°C/+122°F.

The next digit can now be set. Press **READ** until you reach the desired number. Then press **SET** to confirm it. Then the next digit will start flashing. Continue until all digits of the alarm temperature are set.

Setting up a Fahrenheit Temperature Limit of +100°F or Higher


Note: The maximum Celsius temperature is +50°C (internal sensor) respectively +55°C (external sensor). This option is only available for temperatures in Fahrenheit.

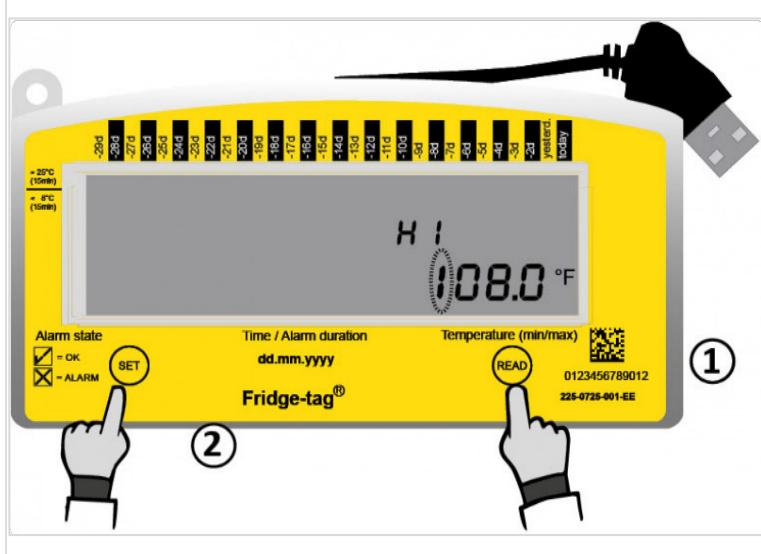

- Press **READ** until a leading "1" is flashing on the display.
- Press **SET** to adjust the limit equal or above +100°F.

The next digit of the temperature starts flashing. Continue until all digits of the alarm temperature limit are set.

Setting up a Negative Temperature Limit Below 0°C/0°F

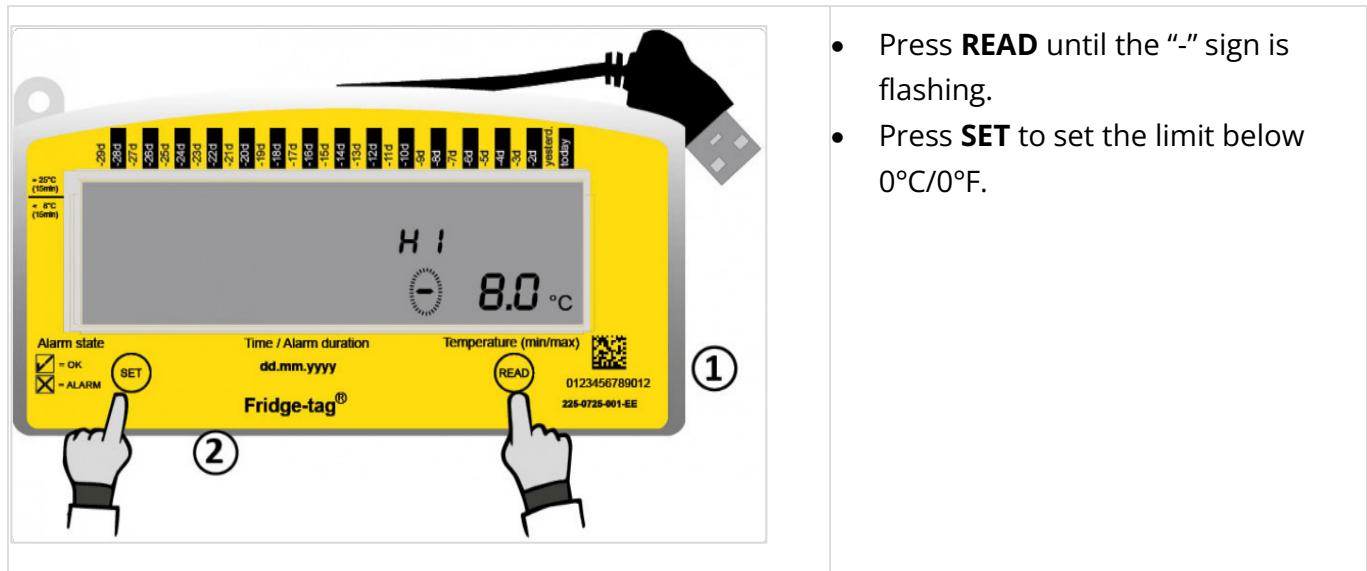

The next digit can now be set.

1. Press **READ** until you reach the desired number.
2. Then press **SET** to confirm it. Then the next digit will start flashing.
3. Continue until all digits of the alarm temperature limits are set.

As soon as the parameters of the upper alarm limit are set, the first digit of the duration of the lower alarm limit will start flashing.

4. Proceed the same way as you did with the upper alarm limit.

As soon as the last digit of the lower alarm limit is confirmed, the activation is completed.

- **Internal sensor:** Now place the Fridge-tag. Refer to section [Placing the Fridge-Tag](#).
- **External sensor:** Connect the device with the external sensor.


Note: In case the desired temperature limit cannot be confirmed, check if the temperature is set within the allowed operating temperature range.

Connection Error (External Sensor Only)

After 10 minutes (factory standard) without a connection between the device and the external sensor the following display appears and:

- The buzzer will beep twice at intervals of three minutes for a maximum of 168 hours (7 days).
- The whole display starts blinking.
- Any button pressed will stop the display from blinking.
- The buzzer only stops if the connection error is corrected. If the error still exists, the buzzer continuously beeps at a three-minute interval for 168 hours (7 days).

Display status: external sensor error.

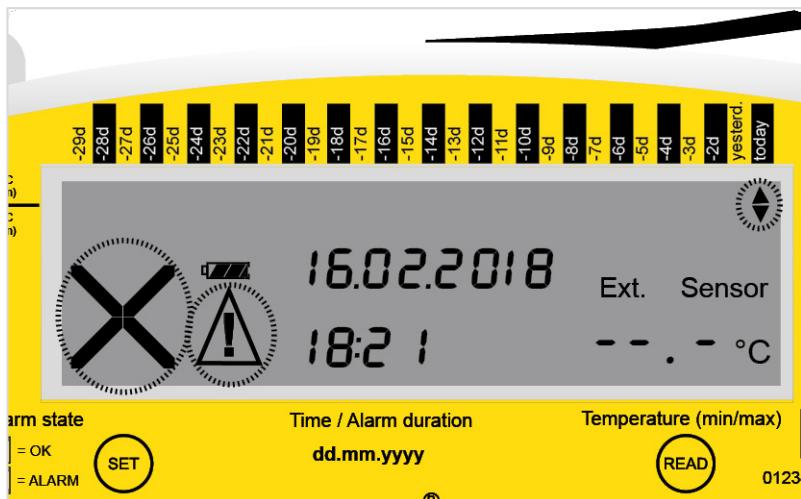


How to Fix the Connection Error

Please check the following two points:

- If the external sensors properly connected with the device?
- Does the external sensor cable have any defects?


Note: As soon as the error(s) have been cleared, the measuring will continue, and the connection error buzzer stops to beep automatically. During max. 1 minute after the connection no temperature is displayed on the screen.

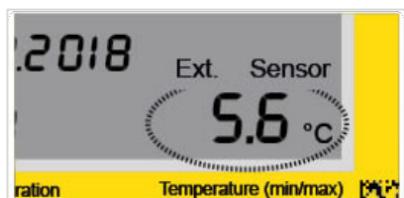

During a connection error no data will be recorded.

Read and Change Settings

Overview: Menu

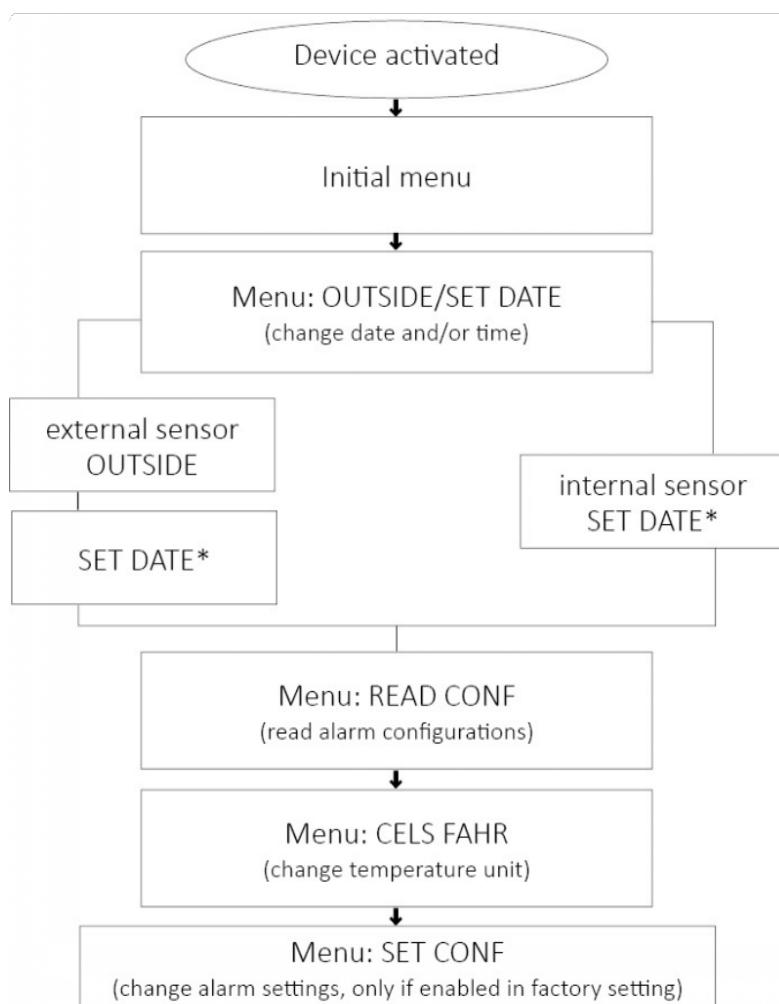


*If "Disable User Clock Adjust" in the configuration is enabled point "SET DATE" are skipped upon activation

Note: If you scroll through the menu and you reach the display of the measuring mode, you need to restart from the beginning by accessing the menu.

In order to adjust more than one setting (e.g. time and Celsius to Fahrenheit) you must complete each change and return to menu mode for the 2nd change.

Initial Menu (Read and Change Settings)

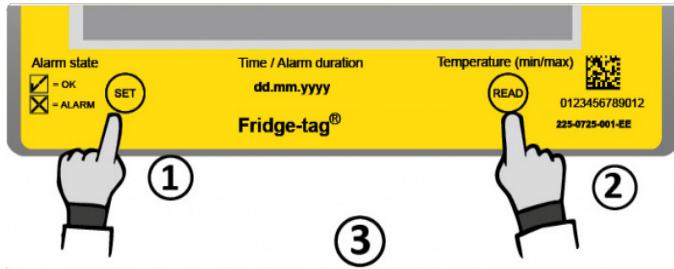

To change the date format, the date, the time, the temperature measurement unit or the alarm settings or to read the preset alarm limits please proceed as follows:

1. Press and hold **SET** ...
2. ... then press **READ** shortly ...
3. ... then release both buttons simultaneously.

- **SET DATE** (internal sensor) is now displayed on the screen.
- **OUTSIDE** (external sensor) is now displayed on the screen.

You entered the menu mode and may choose which entry to see or change.

Menu Access

The following menus are available on sensors:

- **SET DATE**: change date and/or time settings.
- **READ CONF**: read the alarm settings.
- **CELS FAHR**: change the temperature unit.
- **SET CONF**: change the alarm settings (only if enabled in factory setting).

Follow the instructions to access menus:

- **OUTSIDE** (external sensor):
 - first screen shows the temperature measured with the internal sensor of the Fridge-tag (normal ambient temperature).
 - Press **READ** once to get to **SET DATE**.
- **SET DATE** (internal sensor): Configuration with internal sensor.
 - **SET DATE** is directly shown.
 - Use the **READ** button to scroll through the menu.
 - Use the **SET** button to access the corresponding menu.

Access the "SET DATE" Menu

- **External sensor:** The display shows **OUTSIDE**.
 - Press **READ** until the display shows **SET DATE**.
- **Internal sensor:** The display shows the menu **SET DATE**.
 - Press **SET** to access the menu to adjust the date format, date or time settings.
 - Follow the steps in the [Setting the Date](#) and [Setting the Time](#) sections.

Note: Changing the time or date does not affect alarm records. Users can update the date, time, or temperature unit as often as needed. Once activated, the device cannot be turned off. After any change, Fridge-tag locks for 24 hours from midnight after the modification for security (e.g., a change on September 15 triggers a lock from 00:01 am September 16 to 00:01 am September 17).

Access the "READ CONF" Menu

The display shows **SET DATE** (internal sensor), **OUTSIDE** (external sensor).

- Press **READ** until the display shows **READ CONF**.
- Press **SET** to access the menu to read the current alarm configurations. First the display check appears.
- Then press **READ** repeatedly to scroll through the preset alarm parameters.

Access the "CELS FAHR" Menu

The display shows **SET DATE**.

- Press **READ** until the display shows **CELS FAHR**.
- Press **SET** to access the menu to change the temperature measurement unit.
- To change the measurement unit (Celsius/Fahrenheit) press **READ** until the display shows the desired sign (°C/°F).
- Press **SET** to confirm the measurement unit.

Access the "SET CONF" * Menu


The display shows **SET DATE**.

- Press **READ** until the display shows **SET CONF**.
- Press **SET** to access the menu to change the alarm configurations.
- To change the alarm limits (duration or temperature) please refer to the [Setting Alarm Limits \(if preset by factory\)](#) section.

*Changes of the alarm limits are only possible for devices which are programmed with this feature.


Screen Displays During Measurement Mode

Indication for max. 1 minute after completing the activation or after connecting the device with the external sensor. For a maximum of 1 minute no temperature is displayed on the screen, indicated by —. -

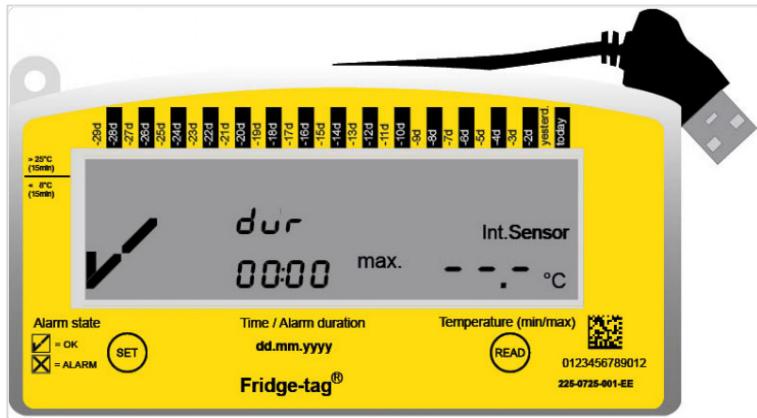


Example OK Display – During Measurement

- Once the device is fully activated the OK symbol ✓, the current temperature reading, the time and the date will be displayed on the screen.
- The Fridge-tag will also indicate whether the measuring is made with an internal sensor or an external sensor.
- The OK symbol ✓ is shown during normal operation as long as no alarms have been recorded. The temperature and time conditions were within the preset alarm limits.

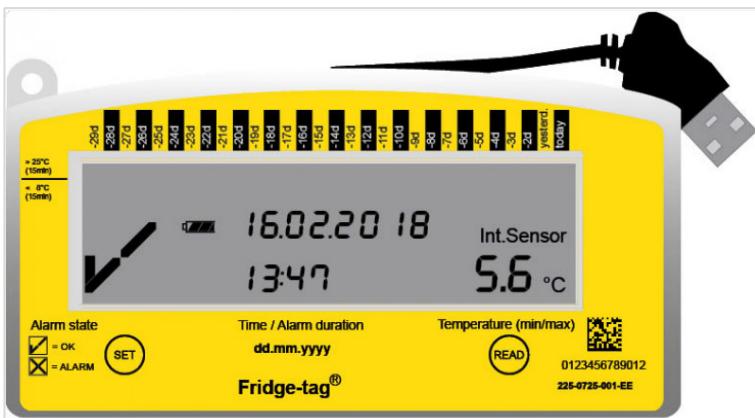

Example Alarm Display – During Measurement

If the preset alarm limits are exceeded, the following information will be displayed on the screen:

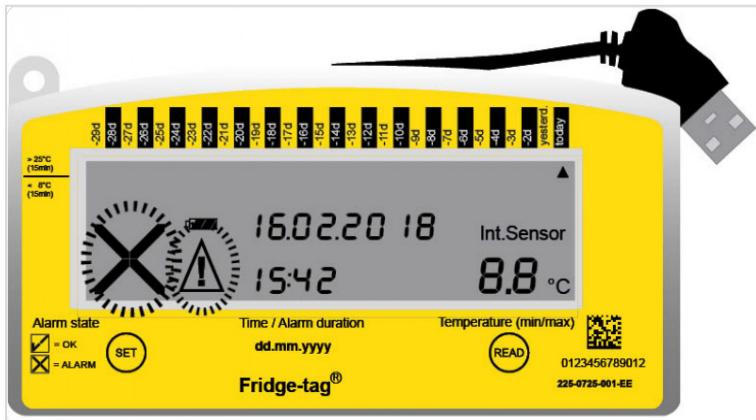

- ✓ (OK symbol) will be replaced by X (alarm symbol)
- An additional alarm indicator ▲ will be indicated in the upper display area to show which alarm limit has been exceeded and on which day.
- In addition to the alarm symbol X the warning symbol Δ will appear next to it.

Alarm Trigger Function

Single-Event Alarm Triggering


The upper or lower alarm triggering is done with a single-event alarm algorithm. Any kind of alarm is triggered if the temperature is continuously out of the preset alarm limits for longer than the preset alarm trigger time.

Upper Alarm Triggering

Setting upper limit: Temperature $>8.0^{\circ}\text{C}$, duration >10 hours.


For the upper alarm to be triggered the temperature needs to be continuously above 8°C for more than 10 hours.

Alarm triggered: alarm symbol \times and warning symbol Δ displayed.

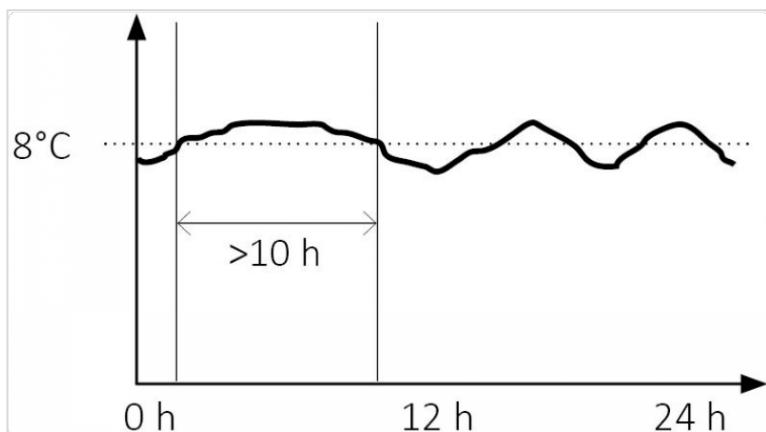

In the example below the sum* of the daily upper temperature deviation is about 20 hours. No alarm will be triggered! The temperature was not continuously out of the preset alarm limits for more than 10 hours in one row.

No Alarm triggered: OK symbol \checkmark on the display.

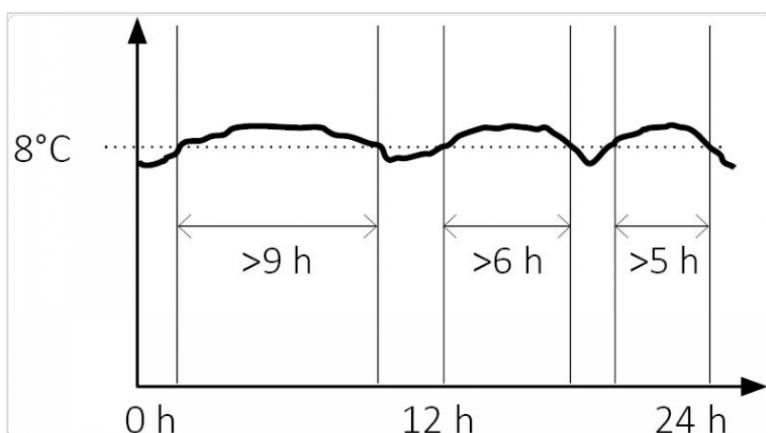


*The sum of the deviations is visible in the daily statistics in the column "Cumulative daily time above the limit."

Lower Alarm Triggering

Setting lower limit: Temperature $<-0.5^{\circ}\text{C}$, duration >1 hour.


For a lower alarm to be triggered the temperature needs to be continuously below -0.5°C for more than 1 hour.

Alarm triggered: alarm symbol \times and warning symbol \triangle displayed.

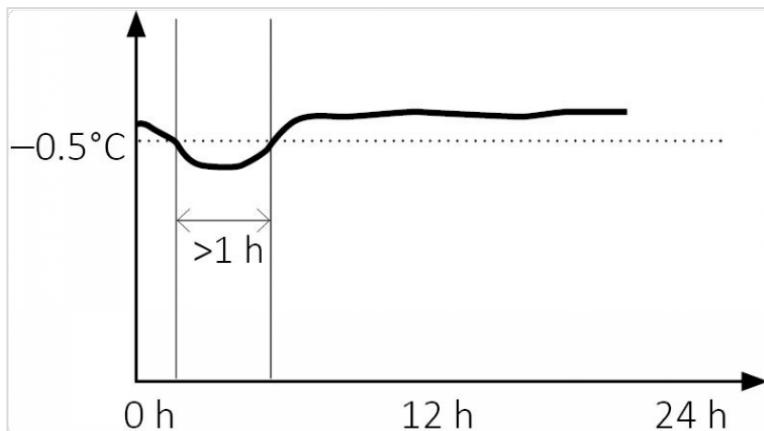

In the example below multiple low temperature deviations* are occurring. No alarm will be triggered. Each temperature deviation was less than 1 hour out of the preset alarm limits.


No Alarm triggered: OK symbol \checkmark on the display.

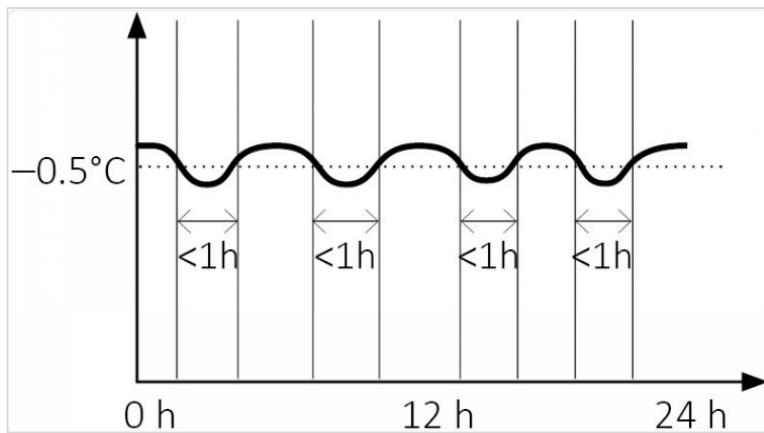


*The sum of the deviations is visible in the daily statistics in the column "Cumulative daily time below the limit."

Alarm Display and Confirmation Options

Option 1: Alarm Indication "All Alarms"

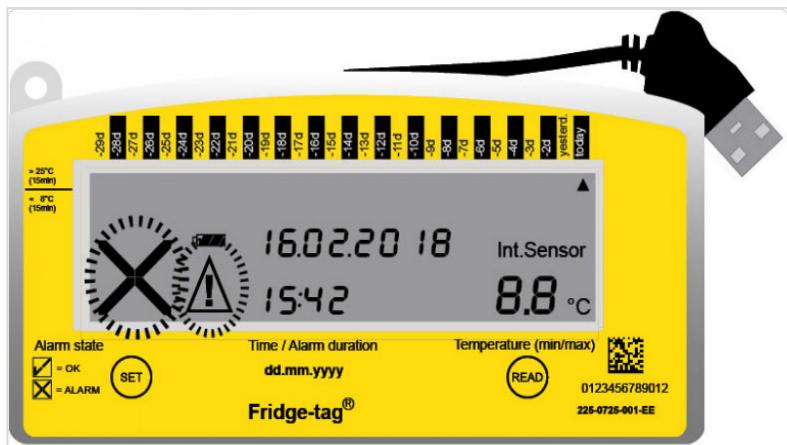

With this option, alarms will be visible on the display with an alarm symbol **X** for 30 days.

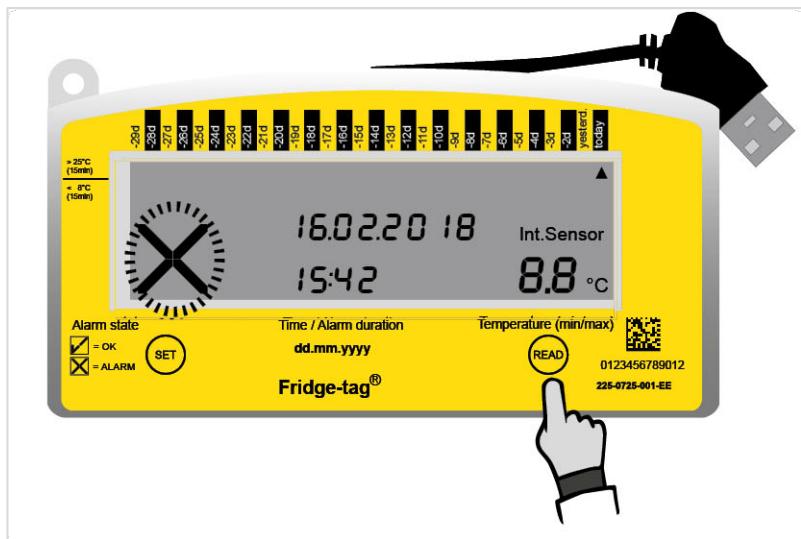



By pressing the **READ** button, the warning symbol **Δ** will be disabled for the corresponding alarms. The alarm symbol **X** cannot be canceled nor reset.

Note:

- In this mode only one upper and one lower alarm will be triggered per day.
- The alarm symbol **X** will be present on the display for 30 days.
- The warning symbol **Δ** can be deactivated by confirming all existing alarms in the readout mode.
- The alarm buzzer stops when the alarm is confirmed within the set alarm limits. Otherwise, the buzzer pauses for approx. 1 hour and starts again for up to 168 hours (7 days).

Option 2: Alarm Indication "Unconfirmed Alarms"

The alarms are shown with the alarm symbol **X** until all alarms (in the 30-day history) have been confirmed as solved by pressing the **READ** button. Afterwards the display will show the OK symbol **✓** until a new alarm is triggered.

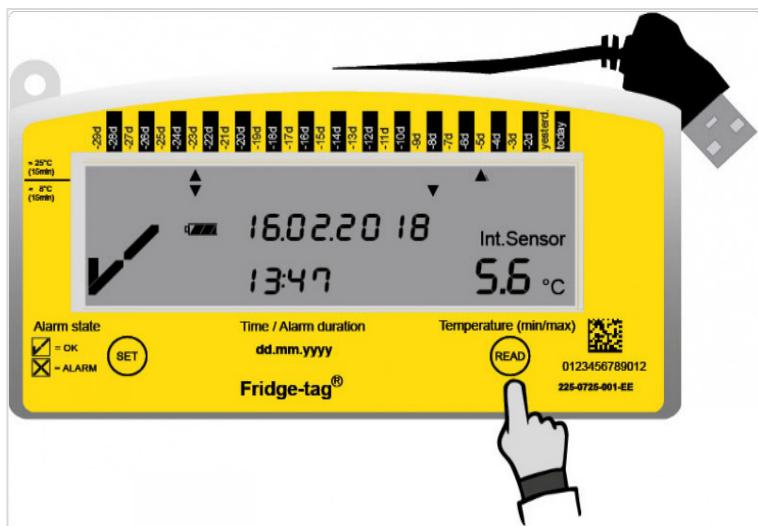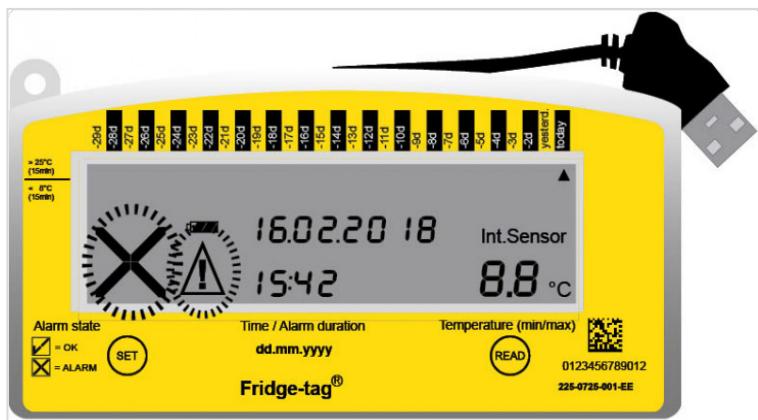


By pressing the **READ** button, the warning symbol **Δ** will be disabled for the corresponding alarms. The alarm symbol **X** disappears and the OK symbol **✓** will be shown again.

Confirmation Options of Currently Triggered Alarms of the Day

1. Device is within the set alarm limits

Press the **READ** button and the alarm symbol **X** and the warning symbol **Δ** will immediately disappear and the optional buzzer stops. A new alarm will be triggered as soon as the set alarm limits are exceeded again.

Settings: upper temperature limit >8.0°C and duration >1-hour, lower temperature limit <-0.5°C and duration 1 hour

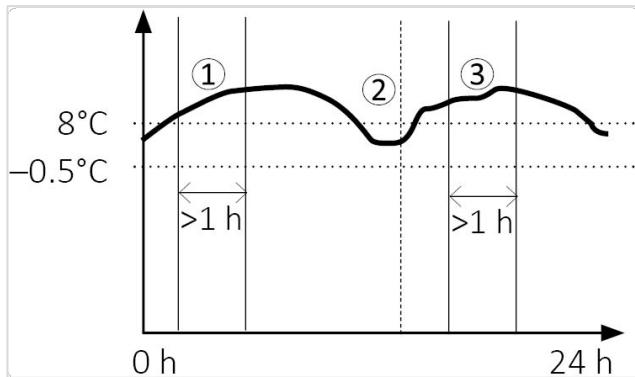


- Alarm triggered: alarm symbol **X** and warning symbol **Δ** on display
- Alarm confirmed within the set temperature limits: **✓** (OK symbol) on display
- Alarm triggered: alarm symbol **X** and warning symbol **Δ** on display.

2. Device is outside the set alarm limits

If the **READ** button is pressed still during a temperature violation the buzzer will be muted for approx. 1 hour. The alarm symbol **X** and the warning symbol **Δ** will stay on display for the corresponding alarm. If the temperature still exceeds the limit after 1 hour, the buzzer will restart beeping.

Settings: upper temperature limit Temperature >8.0°C and duration >1-hour, lower temperature limit <-0.5°C and duration 1 hour:

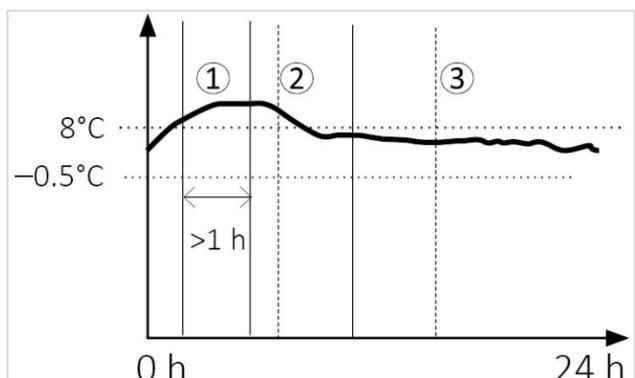

- Alarm triggered: alarm symbol **X** and warning symbol **Δ** on display.
- Alarm confirmed when the temperature exceeds the set temperature limits: alarm symbol **X** and warning symbol **Δ** remain on display.
- Temperature is back within the alarm limits. Now the alarm can be successfully confirmed. OK symbol **✓** on display.


Note: How the alarm symbol **X** and the warning symbol **Δ** react is specified during configuration of the device in the factory settings.

Cumulative Daily Time Above/Below the Limit

The alarm trigger algorithm is based on a single event, although the Fridge-tag is measuring on a daily basis the individual total time above or below the temperature limits. This measurement is not used for any alarm condition. These recordings are only available in the generated PDF/ASCII files.

Note: It could be that the total cumulative time above/below the temperature limits is longer than the configured single-event alarm time without any alarm triggering.

Example setup: lower temperature limit $<-0.5^{\circ}\text{C}$, duration >1 hour:

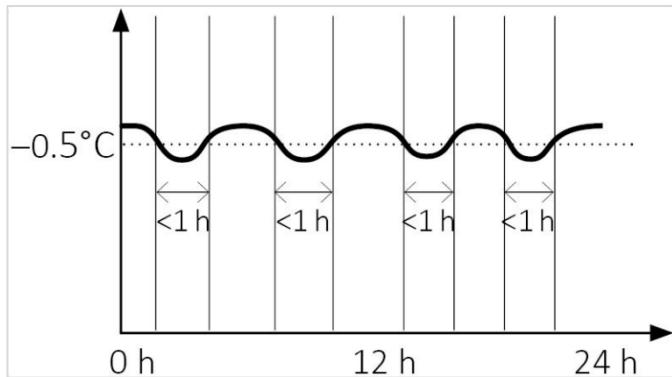

In the above example multiple low temperature deviations with exposure times of less than 1 hour occurred. The cumulative daily time below the limits adds up to about 3.5 hours but no alarm will be triggered. The same behavior also applies to the upper alarm.

Audio Alarm (Optional Factory Setting)

In case an upper or lower alarm is triggered, 3 audible alarm signals are emitted immediately. Thereafter:

- Every minute 1 alarm signal for maximally 168 hours (7 days).
- After 168 hours (7 days) the buzzer will stop.
- If an alarm event is confirmed (READ is pressed) while the limits are still exceeded, the buzzer pauses for approx. 1 hour and then restarts beeping every 3 minutes.
- Confirmation within the alarm limits will stop the buzzer.

In case of a connection error, please refer to the [Connection Error \(External Sensor Only\)](#) section.

Reading History / Readout Mode


The information of the temperature deviations can either be viewed for the past 30 days directly on the device or for 28/56/84/112 days in the generated files (PDF/ASCII).

Note: The external sensor of the Fridge-tag can remain at its location for the readout process. Please consider that there may be a connection error after more than 10 minutes without connection between the device and the sensor.

The Fridge-tag is SmartView compatible.

Option 1: Read From Device (30-Day History)


Example of an OK display during readout of history

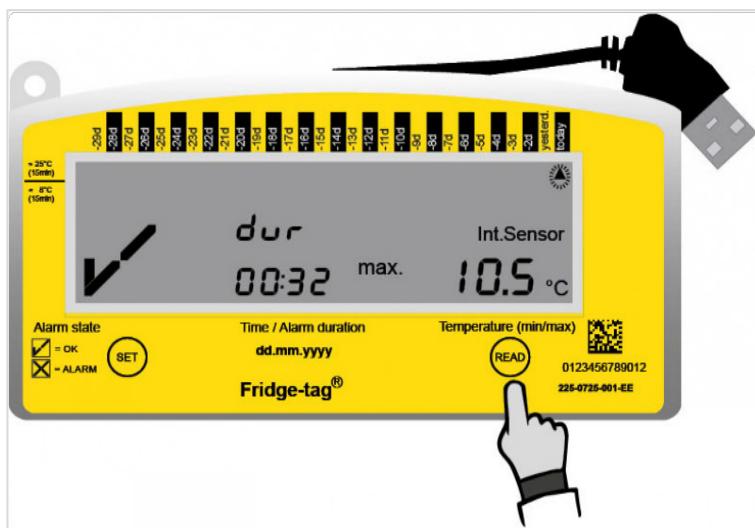

Press **READ** once.

The following information is indicated on the screen:

- The OK symbol ✓.
- The corresponding flashing arrow ▲ (example: high arrow “today”).
- Highest recorded temperature (example: +10.5°C).
- Duration of the exceedance of the preset high limit temperature (example 00:32; hh:min).

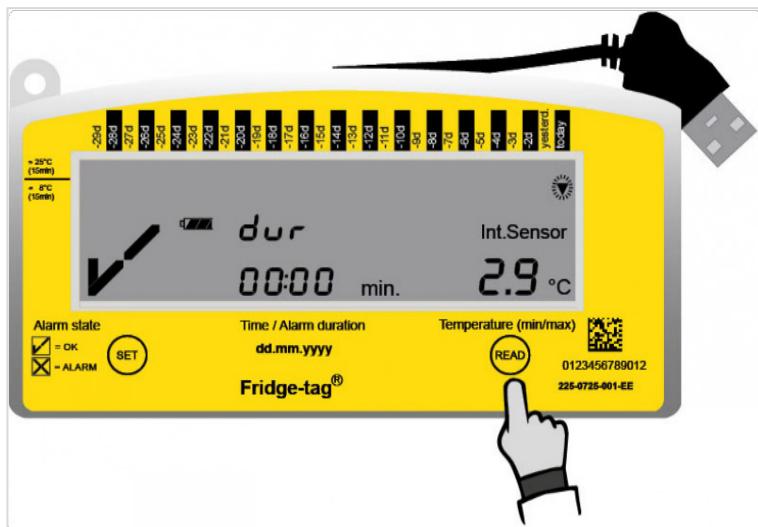

Press **READ** again.

The following information is indicated on the screen:

- The OK symbol ✓.
- The corresponding flashing arrow ▼ (example: low arrow of "today").
- Lowest recorded temperature (example: +2.9°C).
- Duration of the exceedance of the preset low temperature limit (example 00:00; hh:min).


Note: in the Readout mode the flashing arrows display the day where you are (30-day history) and show the highest ▲ and lowest ▼ measured temperature of the corresponding day. If a limit has been exceeded also the duration is shown.

Note: Press repeatedly the READ button to the details of the past 30 days.

When you reach an alarm event, the indication on the screen of the Fridge-tag will be different than the OK display.

Example of an alarm display during readout of history

1st display of a “lower alarm event”:

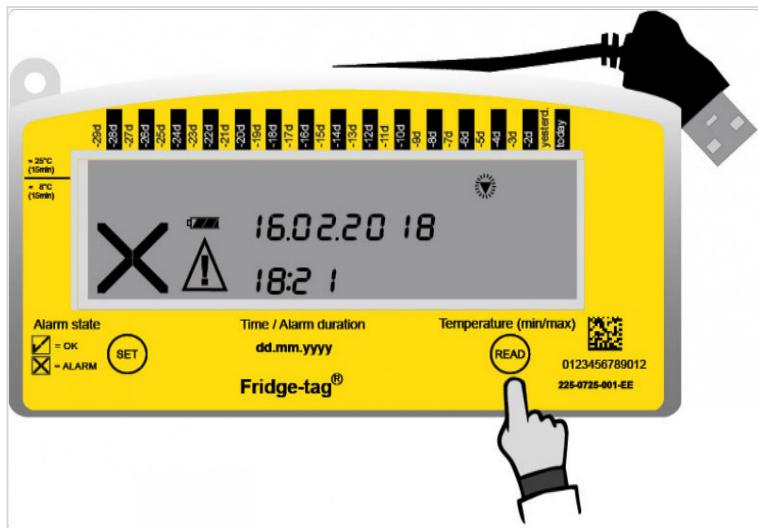


Press **READ** once.

The following information is indicated on the screen:

- The alarm- **X** and the warning symbol **⚠**.
- The corresponding alarm indicator **▼** (lower alarm limit).
- Day of alarm (example: 5 days ago: -5d).
- The date of the alarm (example: 16.02.2018).
- The time of the alarm (example: 18:21).

2nd display of a “lower alarm event”:

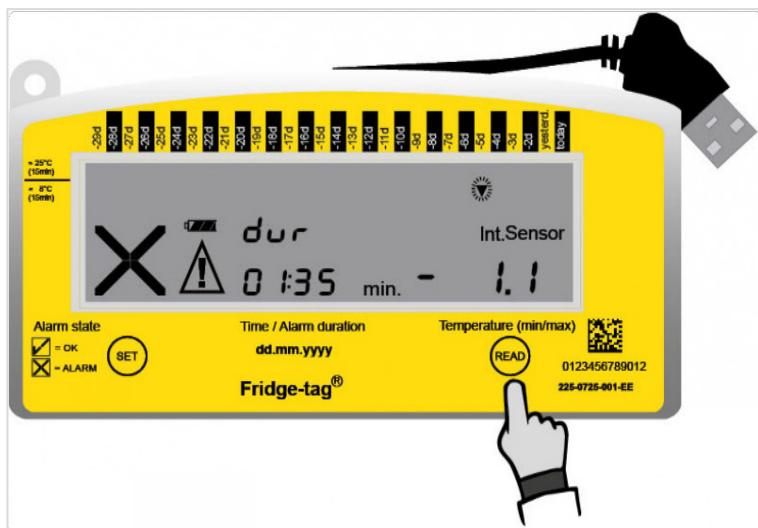


Press **READ** a second time.

The following additional information is indicated on the screen:

- Lowest recorded temperature (example: -1.1°C).
- The duration of the exceedance of the preset low temperature limit (example: 01:35; hh:mm).
- Temperature recording in this example with internal sensor.

Option 2: Read Alarms on the Device (Alarm Super Jump Function)

1st display of the latest alarm events:

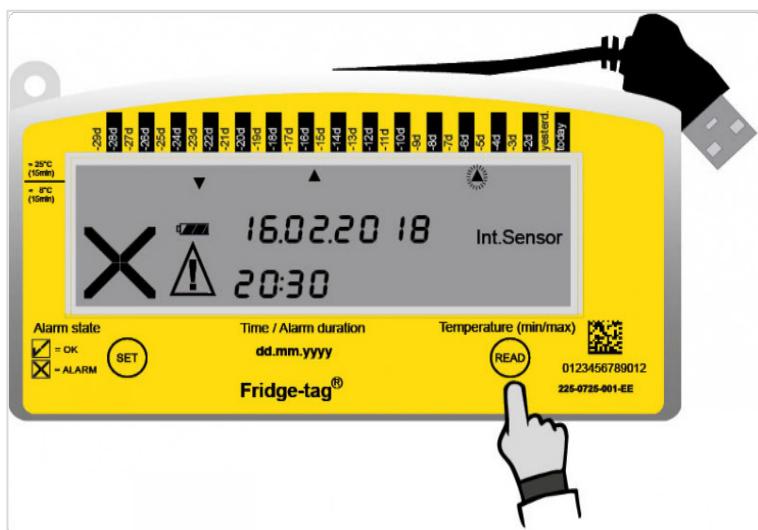


Press the **READ** button for at least 3 seconds.

The following information is indicated on the screen:

- The alarm symbol **X** and the warning symbol **⚠**
- The corresponding alarm indicator **▲** (higher alarm limit)
- Day of alarm (example: 5 days ago: -5d)
- The date of the alarm (example: 16.02.2018)
- The time of excursion (example: 20:30)

2nd display of the latest alarm events:

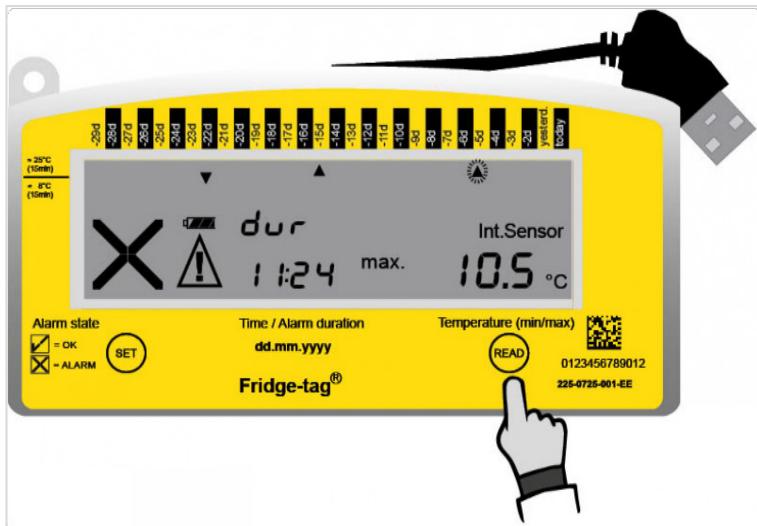


Press **READ** again.

The following additional information is indicated on the screen:

- Highest recorded temperature (example: +10.5°C)
- The duration of the exceedance of the preset high temperature limit (example: 11:24; hh:mm).
- Temperature recording in this example with internal sensor

Note: Press the **READ** button again for at least 3 seconds and the next alarm event will appear on the screen.

Display of the next alarm event:

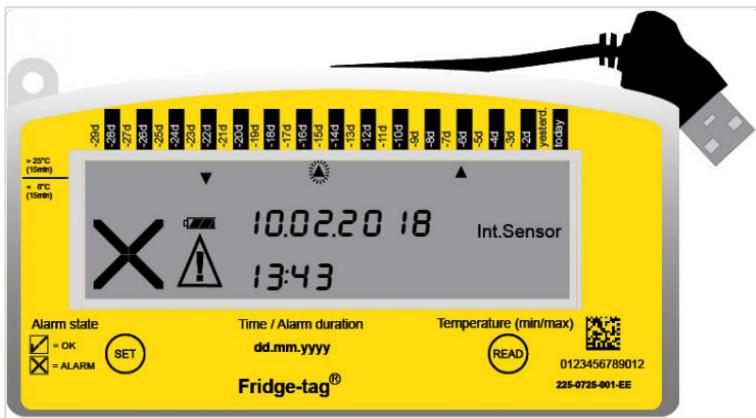


- Press the **READ** button again for 3 seconds to jump to the next alarm event.
- Press **SET** in the "Read out Mode" to return to the "Measurement Mode."

Option 3: Read Data from the Files Generated by the Fridge-Tag

Plug the Fridge-tag into any computer via USB interface. Make sure the device is plugged in properly.

Note: Disconnect the external sensor from the device first.

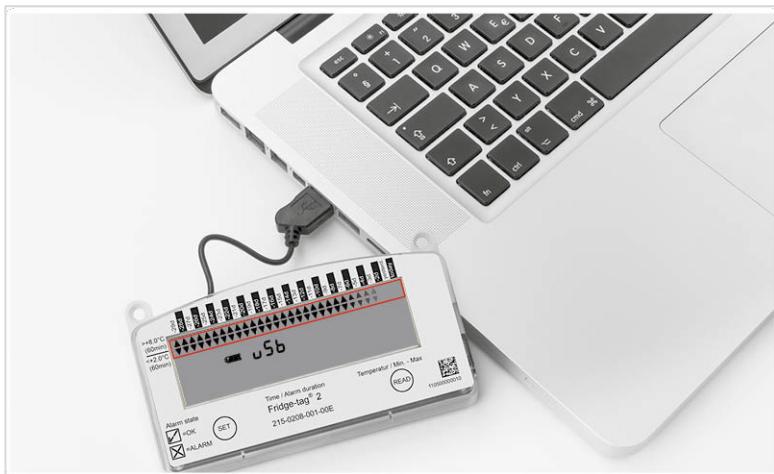


The Fridge-tag will now generate a PDF and ASCII report of the last 28, 56, 84 or 112 days (factory setting). Depending on the configuration, this process may take up to 2 minutes.

Choose the appropriate file generated by the Fridge-tag.

USB connection of the Fridge-tag


The continuously appearing arrows in the upper display area indicate that the device is operating.

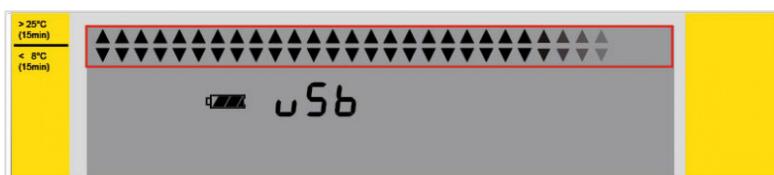


Note: This process must not be interrupted until the OK symbol appears on the display. This indicates that the creation of the ASCII and PDF files has been successfully completed.




The hard drive of the Fridge-tag is shown in your explorer. Open the desired file generated by the device.

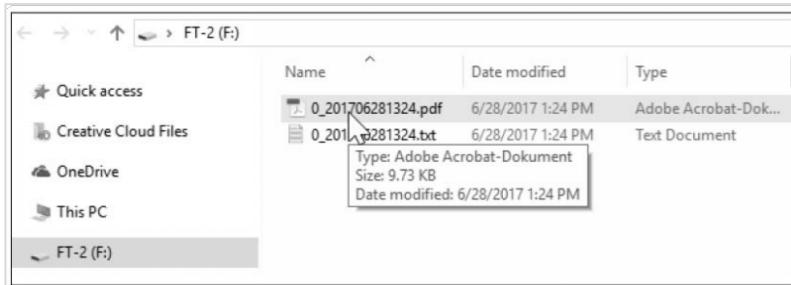

Note: To disconnect the device properly, please always use the function "Safely Remove Hardware" on your PC/Mac.

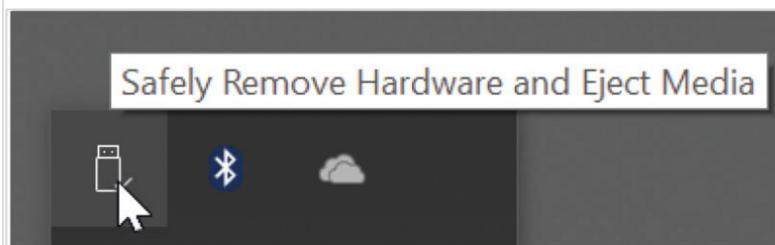

- Right-click the icon "Safely Remove Hardware and Eject Media" in the Windows taskbar (lower right corner).
- Choose the corresponding device to remove.

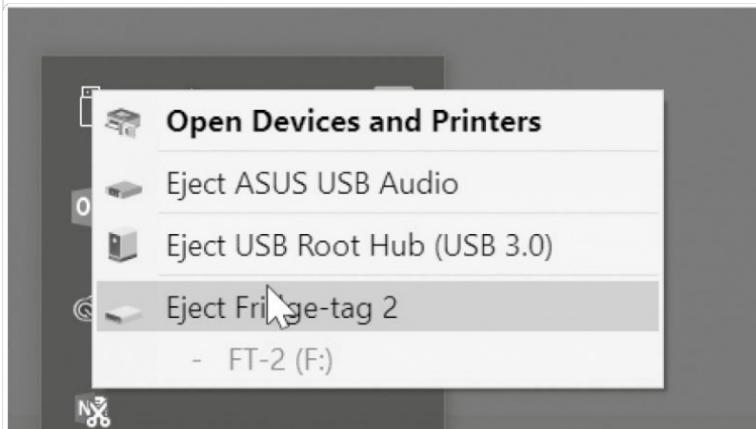

Do not disconnect the device before you receive the depicted message, otherwise the device can be damaged.

Note: For this process no additional software is necessary.


PDF Report Explanation

The following is a sample of a PDF file generated by a Fridge-tag 2 L with external sensor (page 1/2):

<p>① PDF document of the Fridge-tag</p> <p>② Identification number: 510500000006 Date and time of report creation: 12/10/2017 20:37h Activation date: 01/05/2018 13:40h</p> <p>③ Upper alarm limit: Above +8.0°C for 1 min Lower alarm limit: Below +2.0°C for 1 min</p> <p>④ Measurement interval:¹⁾ 1min (fixed) Logging interval: 5min</p>																																																																																																																																																																																																																																																																																																																																																																																																																																											
<p>⑩ Time zone: UTC+01:00 ⑪ Low battery since: 12/25/2017</p>																																																																																																																																																																																																																																																																																																																																																																																																																																											
<p>⑤</p>																																																																																																																																																																																																																																																																																																																																																																																																																																											
<table border="1"> <thead> <tr> <th rowspan="2">No.</th> <th rowspan="2">Date (MM/dd/yyyy)</th> <th rowspan="2">Events²⁾</th> <th rowspan="2">Average temp.</th> <th colspan="3">Lower alarm limit</th> <th colspan="3">Upper alarm limit</th> <th colspan="3">Ext. sensor connection error</th> </tr> <tr> <th>Status</th> <th>Min. temp.</th> <th>Cumulative daily time below the limit</th> <th>Alarm trigger time</th> <th>Status</th> <th>Max. temp.</th> <th>Cumulative daily time above the limit</th> <th>Alarm trigger time</th> <th>Status</th> <th>Duration</th> <th>Alarm trigger time</th> </tr> </thead> <tbody> <tr><td>1</td><td>Today</td><td></td><td>+1.8°C</td><td>ALARM!!</td><td>-1.0°C</td><td>11h 4min</td><td>00:00h</td><td>In progress</td><td>+5.8°C</td><td>0min</td><td>In progress</td><td>23h 59min</td><td>08.27h</td></tr> <tr><td>2</td><td>01/05/2018</td><td></td><td>+1.5°C</td><td>ALARM!!</td><td>-0.8°C</td><td>17h 29min</td><td>00:00h</td><td>ok</td><td>+5.7°C</td><td>0min</td><td>ok</td><td>0min</td><td></td></tr> <tr><td>3</td><td>01/04/2018</td><td></td><td>+1.5°C</td><td>ALARM!!</td><td>-1.0°C</td><td>16h 1min</td><td>00:26h</td><td>ok</td><td>+4.5°C</td><td>0min</td><td>ok</td><td>0min</td><td></td></tr> <tr><td>4</td><td>01/03/2018</td><td></td><td>+2.0°C</td><td>ALARM!!</td><td>-0.5°C</td><td>16h 1min</td><td>00:00h</td><td>ok</td><td>+6.4°C</td><td>0min</td><td>ok</td><td>0min</td><td></td></tr> <tr><td>5</td><td>01/02/2018</td><td></td><td>+1.7°C</td><td>ALARM!!</td><td>-1.4°C</td><td>14h 44min</td><td>00:00h</td><td>ok</td><td>+7.5°C</td><td>0min</td><td>ok</td><td>0min</td><td></td></tr> <tr><td>6</td><td>01/01/2018</td><td></td><td>+2.3°C</td><td>ALARM!!</td><td>-0.7°C</td><td>9h 35min</td><td>06:19h</td><td>ok</td><td>+6.5°C</td><td>0min</td><td>ok</td><td>0min</td><td></td></tr> <tr><td>7</td><td>12/31/2017</td><td></td><td>+0.9°C</td><td>ALARM!!</td><td>-5.3°C</td><td>9h 24min</td><td>00:00h</td><td>ok</td><td>+5.3°C</td><td>0min</td><td>ok</td><td>0min</td><td></td></tr> <tr><td>8</td><td>12/30/2017</td><td></td><td>-1.7°C</td><td>ALARM!!</td><td>-5.1°C</td><td>22h 46min</td><td>00:1h</td><td>ok</td><td>+2.5°C</td><td>0min</td><td>ok</td><td>0min</td><td></td></tr> <tr><td>9</td><td>12/29/2017</td><td></td><td>-0.9°C</td><td>ALARM!!</td><td>-4.2°C</td><td>13h 22min</td><td>00:00h</td><td>ALARM!!</td><td>+6.5°C</td><td>14min</td><td>13:48h</td><td>ok</td><td>0min</td></tr> <tr><td>10</td><td>12/28/2017</td><td></td><td>-0.3°C</td><td>ALARM!!</td><td>-3.4°C</td><td>20h 1min</td><td>00:00h</td><td>ok</td><td>+6.0°C</td><td>0min</td><td>ok</td><td>0min</td><td></td></tr> <tr><td>11</td><td>12/27/2017</td><td></td><td>+0.0°C</td><td>ALARM!!</td><td>-2.9°C</td><td>19h 42min</td><td>00:00h</td><td>ok</td><td>+5.9°C</td><td>0min</td><td>ok</td><td>0min</td><td></td></tr> <tr><td>12</td><td>12/26/2017</td><td></td><td>+0.0°C</td><td>ALARM!!</td><td>-2.2°C</td><td>19h 47min</td><td>00:00h</td><td>ok</td><td>+6.4°C</td><td>0min</td><td>ok</td><td>0min</td><td></td></tr> <tr><td>13</td><td>12/25/2017</td><td></td><td>+2.3°C</td><td>ALARM!!</td><td>-0.5°C</td><td>13h 19min</td><td>02:28h</td><td>ALARM!!</td><td>+6.3°C</td><td>24min</td><td>12:51h</td><td>ok</td><td>0min</td></tr> <tr><td>14</td><td>12/24/2017</td><td></td><td>+2.4°C</td><td>ALARM!!</td><td>-1.2°C</td><td>1h 14min</td><td>00:00h</td><td>ALARM!!</td><td>+6.6°C</td><td>30min</td><td>10:59h</td><td>ok</td><td>0min</td></tr> <tr><td>15</td><td>12/23/2017</td><td></td><td>+3.3°C</td><td>ALARM!!</td><td>-1.3°C</td><td>10h 34min</td><td>00:00h</td><td>ALARM!!</td><td>+11.0°C</td><td>2h 55min</td><td>12:05h</td><td>ok</td><td>0min</td></tr> <tr><td>16</td><td>12/22/2017</td><td>a. 19:35</td><td>+3.3°C</td><td>ALARM</td><td>-0.5°C</td><td>7h 25min</td><td>06:37h</td><td>ALARM</td><td>+6.2°C</td><td>13min</td><td>12:53h</td><td>ok</td><td>0min</td></tr> <tr><td>17</td><td>12/21/2017</td><td></td><td>+5.0°C</td><td>ALARM</td><td>+1.7°C</td><td>38min</td><td>22:41h</td><td>ALARM</td><td>+6.3°C</td><td>32min</td><td>09:30h</td><td>ok</td><td>0min</td></tr> <tr><td>18</td><td>12/20/2017</td><td></td><td>+3.1°C</td><td>ALARM</td><td>+0.3°C</td><td>10h 32min</td><td>00:00h</td><td>ALARM</td><td>+10.2°C</td><td>2h 38min</td><td>11:27h</td><td>ok</td><td>0min</td></tr> <tr><td>19</td><td>12/19/2017</td><td></td><td>+4.0°C</td><td>ALARM</td><td>+0.7°C</td><td>7h 33min</td><td>05:36h</td><td>ALARM</td><td>+6.3°C</td><td>3h 4min</td><td>10:29h</td><td>ok</td><td>0min</td></tr> <tr><td>20</td><td>12/18/2017</td><td></td><td>+5.4°C</td><td>ALARM</td><td>+0.4°C</td><td>4h 9min</td><td>00:00h</td><td>ALARM</td><td>+10.8°C</td><td>4h 54min</td><td>10:03h</td><td>ok</td><td>0min</td></tr> <tr><td>21</td><td>12/17/2017</td><td></td><td>+4.6°C</td><td>ALARM</td><td>+1.1°C</td><td>3h 18min</td><td>18:54h</td><td>ALARM</td><td>+6.8°C</td><td>1h 38min</td><td>11:57h</td><td>ok</td><td>0min</td></tr> <tr><td>22</td><td>12/16/2017</td><td></td><td>+5.3°C</td><td>ALARM</td><td>+1.9°C</td><td>3min</td><td>00:1h</td><td>ALARM</td><td>+9.0°C</td><td>1h 14min</td><td>11:43h</td><td>ok</td><td>0min</td></tr> <tr><td>23</td><td>12/15/2017</td><td></td><td>+0.5°C</td><td>ALARM</td><td>-2.8°C</td><td>14h 59min</td><td>00:00h</td><td>ok</td><td>+5.1°C</td><td>0min</td><td>ok</td><td>0min</td><td></td></tr> <tr><td>24</td><td>12/14/2017</td><td></td><td>-1.2°C</td><td>ALARM</td><td>-4.1°C</td><td>20h 57min</td><td>00:1h</td><td>ok</td><td>+4.1°C</td><td>0min</td><td>ok</td><td>0min</td><td></td></tr> <tr><td>25</td><td>12/13/2017</td><td></td><td>-2.1°C</td><td>ALARM</td><td>-5.7°C</td><td>21h 53min</td><td>00:00h</td><td>ok</td><td>+3.1°C</td><td>0min</td><td>ok</td><td>0min</td><td></td></tr> <tr><td>26</td><td>12/12/2017</td><td></td><td>+0.3°C</td><td>ALARM</td><td>-4.5°C</td><td>16h 1min</td><td>00:00h</td><td>ok</td><td>+5.1°C</td><td>0min</td><td>ok</td><td>0min</td><td></td></tr> <tr><td>27</td><td>12/11/2017</td><td></td><td>-0.5°C</td><td>ALARM</td><td>-1.7°C</td><td>5h 34min</td><td>18:27h</td><td>ok</td><td>+1.4°C</td><td>0min</td><td>ALARM</td><td>18h 26min</td><td>00:00h</td></tr> <tr><td>28</td><td>12/10/2017</td><td></td><td>+26.0°C</td><td>ok</td><td>+25.3°C</td><td>0min</td><td></td><td>ALARM</td><td>+27.5°C</td><td>2h 20min</td><td>13:42h</td><td>ALARM</td><td>8h</td><td>16:19h</td></tr> </tbody> </table>											No.	Date (MM/dd/yyyy)	Events ²⁾	Average temp.	Lower alarm limit			Upper alarm limit			Ext. sensor connection error			Status	Min. temp.	Cumulative daily time below the limit	Alarm trigger time	Status	Max. temp.	Cumulative daily time above the limit	Alarm trigger time	Status	Duration	Alarm trigger time	1	Today		+1.8°C	ALARM!!	-1.0°C	11h 4min	00:00h	In progress	+5.8°C	0min	In progress	23h 59min	08.27h	2	01/05/2018		+1.5°C	ALARM!!	-0.8°C	17h 29min	00:00h	ok	+5.7°C	0min	ok	0min		3	01/04/2018		+1.5°C	ALARM!!	-1.0°C	16h 1min	00:26h	ok	+4.5°C	0min	ok	0min		4	01/03/2018		+2.0°C	ALARM!!	-0.5°C	16h 1min	00:00h	ok	+6.4°C	0min	ok	0min		5	01/02/2018		+1.7°C	ALARM!!	-1.4°C	14h 44min	00:00h	ok	+7.5°C	0min	ok	0min		6	01/01/2018		+2.3°C	ALARM!!	-0.7°C	9h 35min	06:19h	ok	+6.5°C	0min	ok	0min		7	12/31/2017		+0.9°C	ALARM!!	-5.3°C	9h 24min	00:00h	ok	+5.3°C	0min	ok	0min		8	12/30/2017		-1.7°C	ALARM!!	-5.1°C	22h 46min	00:1h	ok	+2.5°C	0min	ok	0min		9	12/29/2017		-0.9°C	ALARM!!	-4.2°C	13h 22min	00:00h	ALARM!!	+6.5°C	14min	13:48h	ok	0min	10	12/28/2017		-0.3°C	ALARM!!	-3.4°C	20h 1min	00:00h	ok	+6.0°C	0min	ok	0min		11	12/27/2017		+0.0°C	ALARM!!	-2.9°C	19h 42min	00:00h	ok	+5.9°C	0min	ok	0min		12	12/26/2017		+0.0°C	ALARM!!	-2.2°C	19h 47min	00:00h	ok	+6.4°C	0min	ok	0min		13	12/25/2017		+2.3°C	ALARM!!	-0.5°C	13h 19min	02:28h	ALARM!!	+6.3°C	24min	12:51h	ok	0min	14	12/24/2017		+2.4°C	ALARM!!	-1.2°C	1h 14min	00:00h	ALARM!!	+6.6°C	30min	10:59h	ok	0min	15	12/23/2017		+3.3°C	ALARM!!	-1.3°C	10h 34min	00:00h	ALARM!!	+11.0°C	2h 55min	12:05h	ok	0min	16	12/22/2017	a. 19:35	+3.3°C	ALARM	-0.5°C	7h 25min	06:37h	ALARM	+6.2°C	13min	12:53h	ok	0min	17	12/21/2017		+5.0°C	ALARM	+1.7°C	38min	22:41h	ALARM	+6.3°C	32min	09:30h	ok	0min	18	12/20/2017		+3.1°C	ALARM	+0.3°C	10h 32min	00:00h	ALARM	+10.2°C	2h 38min	11:27h	ok	0min	19	12/19/2017		+4.0°C	ALARM	+0.7°C	7h 33min	05:36h	ALARM	+6.3°C	3h 4min	10:29h	ok	0min	20	12/18/2017		+5.4°C	ALARM	+0.4°C	4h 9min	00:00h	ALARM	+10.8°C	4h 54min	10:03h	ok	0min	21	12/17/2017		+4.6°C	ALARM	+1.1°C	3h 18min	18:54h	ALARM	+6.8°C	1h 38min	11:57h	ok	0min	22	12/16/2017		+5.3°C	ALARM	+1.9°C	3min	00:1h	ALARM	+9.0°C	1h 14min	11:43h	ok	0min	23	12/15/2017		+0.5°C	ALARM	-2.8°C	14h 59min	00:00h	ok	+5.1°C	0min	ok	0min		24	12/14/2017		-1.2°C	ALARM	-4.1°C	20h 57min	00:1h	ok	+4.1°C	0min	ok	0min		25	12/13/2017		-2.1°C	ALARM	-5.7°C	21h 53min	00:00h	ok	+3.1°C	0min	ok	0min		26	12/12/2017		+0.3°C	ALARM	-4.5°C	16h 1min	00:00h	ok	+5.1°C	0min	ok	0min		27	12/11/2017		-0.5°C	ALARM	-1.7°C	5h 34min	18:27h	ok	+1.4°C	0min	ALARM	18h 26min	00:00h	28	12/10/2017		+26.0°C	ok	+25.3°C	0min		ALARM	+27.5°C	2h 20min	13:42h	ALARM	8h	16:19h
No.	Date (MM/dd/yyyy)	Events ²⁾	Average temp.	Lower alarm limit			Upper alarm limit			Ext. sensor connection error																																																																																																																																																																																																																																																																																																																																																																																																																																	
				Status	Min. temp.	Cumulative daily time below the limit	Alarm trigger time	Status	Max. temp.	Cumulative daily time above the limit	Alarm trigger time	Status	Duration	Alarm trigger time																																																																																																																																																																																																																																																																																																																																																																																																																													
1	Today		+1.8°C	ALARM!!	-1.0°C	11h 4min	00:00h	In progress	+5.8°C	0min	In progress	23h 59min	08.27h																																																																																																																																																																																																																																																																																																																																																																																																																														
2	01/05/2018		+1.5°C	ALARM!!	-0.8°C	17h 29min	00:00h	ok	+5.7°C	0min	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																															
3	01/04/2018		+1.5°C	ALARM!!	-1.0°C	16h 1min	00:26h	ok	+4.5°C	0min	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																															
4	01/03/2018		+2.0°C	ALARM!!	-0.5°C	16h 1min	00:00h	ok	+6.4°C	0min	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																															
5	01/02/2018		+1.7°C	ALARM!!	-1.4°C	14h 44min	00:00h	ok	+7.5°C	0min	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																															
6	01/01/2018		+2.3°C	ALARM!!	-0.7°C	9h 35min	06:19h	ok	+6.5°C	0min	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																															
7	12/31/2017		+0.9°C	ALARM!!	-5.3°C	9h 24min	00:00h	ok	+5.3°C	0min	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																															
8	12/30/2017		-1.7°C	ALARM!!	-5.1°C	22h 46min	00:1h	ok	+2.5°C	0min	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																															
9	12/29/2017		-0.9°C	ALARM!!	-4.2°C	13h 22min	00:00h	ALARM!!	+6.5°C	14min	13:48h	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																														
10	12/28/2017		-0.3°C	ALARM!!	-3.4°C	20h 1min	00:00h	ok	+6.0°C	0min	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																															
11	12/27/2017		+0.0°C	ALARM!!	-2.9°C	19h 42min	00:00h	ok	+5.9°C	0min	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																															
12	12/26/2017		+0.0°C	ALARM!!	-2.2°C	19h 47min	00:00h	ok	+6.4°C	0min	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																															
13	12/25/2017		+2.3°C	ALARM!!	-0.5°C	13h 19min	02:28h	ALARM!!	+6.3°C	24min	12:51h	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																														
14	12/24/2017		+2.4°C	ALARM!!	-1.2°C	1h 14min	00:00h	ALARM!!	+6.6°C	30min	10:59h	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																														
15	12/23/2017		+3.3°C	ALARM!!	-1.3°C	10h 34min	00:00h	ALARM!!	+11.0°C	2h 55min	12:05h	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																														
16	12/22/2017	a. 19:35	+3.3°C	ALARM	-0.5°C	7h 25min	06:37h	ALARM	+6.2°C	13min	12:53h	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																														
17	12/21/2017		+5.0°C	ALARM	+1.7°C	38min	22:41h	ALARM	+6.3°C	32min	09:30h	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																														
18	12/20/2017		+3.1°C	ALARM	+0.3°C	10h 32min	00:00h	ALARM	+10.2°C	2h 38min	11:27h	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																														
19	12/19/2017		+4.0°C	ALARM	+0.7°C	7h 33min	05:36h	ALARM	+6.3°C	3h 4min	10:29h	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																														
20	12/18/2017		+5.4°C	ALARM	+0.4°C	4h 9min	00:00h	ALARM	+10.8°C	4h 54min	10:03h	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																														
21	12/17/2017		+4.6°C	ALARM	+1.1°C	3h 18min	18:54h	ALARM	+6.8°C	1h 38min	11:57h	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																														
22	12/16/2017		+5.3°C	ALARM	+1.9°C	3min	00:1h	ALARM	+9.0°C	1h 14min	11:43h	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																														
23	12/15/2017		+0.5°C	ALARM	-2.8°C	14h 59min	00:00h	ok	+5.1°C	0min	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																															
24	12/14/2017		-1.2°C	ALARM	-4.1°C	20h 57min	00:1h	ok	+4.1°C	0min	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																															
25	12/13/2017		-2.1°C	ALARM	-5.7°C	21h 53min	00:00h	ok	+3.1°C	0min	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																															
26	12/12/2017		+0.3°C	ALARM	-4.5°C	16h 1min	00:00h	ok	+5.1°C	0min	ok	0min																																																																																																																																																																																																																																																																																																																																																																																																																															
27	12/11/2017		-0.5°C	ALARM	-1.7°C	5h 34min	18:27h	ok	+1.4°C	0min	ALARM	18h 26min	00:00h																																																																																																																																																																																																																																																																																																																																																																																																																														
28	12/10/2017		+26.0°C	ok	+25.3°C	0min		ALARM	+27.5°C	2h 20min	13:42h	ALARM	8h	16:19h																																																																																																																																																																																																																																																																																																																																																																																																																													
<p>⑥ Test String 1 Test String 2 Test String 3</p>																																																																																																																																																																																																																																																																																																																																																																																																																																											
<p>⑦</p>																																																																																																																																																																																																																																																																																																																																																																																																																																											
<p>⑧ 1) Damping and data analysis every minute 2) 1 = time / date changed, a = alarm configuration changed, hh:mm = status checked</p>																																																																																																																																																																																																																																																																																																																																																																																																																																											
<p>⑨ Date and place: _____ Signature: _____</p>																																																																																																																																																																																																																																																																																																																																																																																																																																											

1. Document title and device type
2. Device ID and further information
3. Alarm settings
4. Measuring and logging interval
5. Event and alarm table (latest info in line 1, top line)
6. Up to 3 user-defined strings (max. 30 characters each). Factory preset.
7. Placeholder for notes
8. Notes:
 - Note 1: Reference for measurement interval.
 - Note 2: Legend for events column (hh:mm → 1 time stamp/half day).
9. Placeholder for date/place and signature
10. Time zone
11. Battery warning with timestamp


The following is a sample of a PDF file generated by a Fridge-tag 2 L with external sensor (page 2/2)

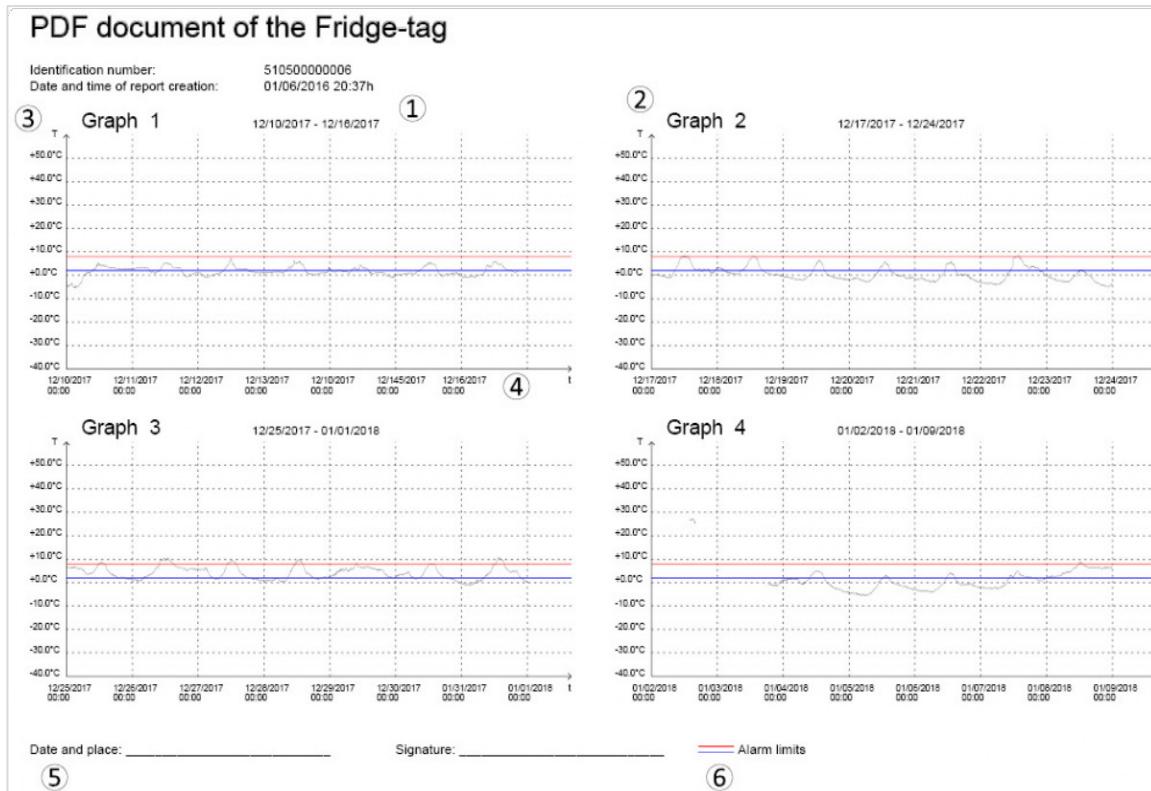

1. Each graph shows data from a period of 7 days.
2. Incrementally numbered graphs.
3. Temperature scale.
4. Time scale.
5. Placeholder for date/place and signature.
6. Alarm limits.

The following is a sample of a graph behavior when date / time is changed manually

PDF document of the Fridge-tag

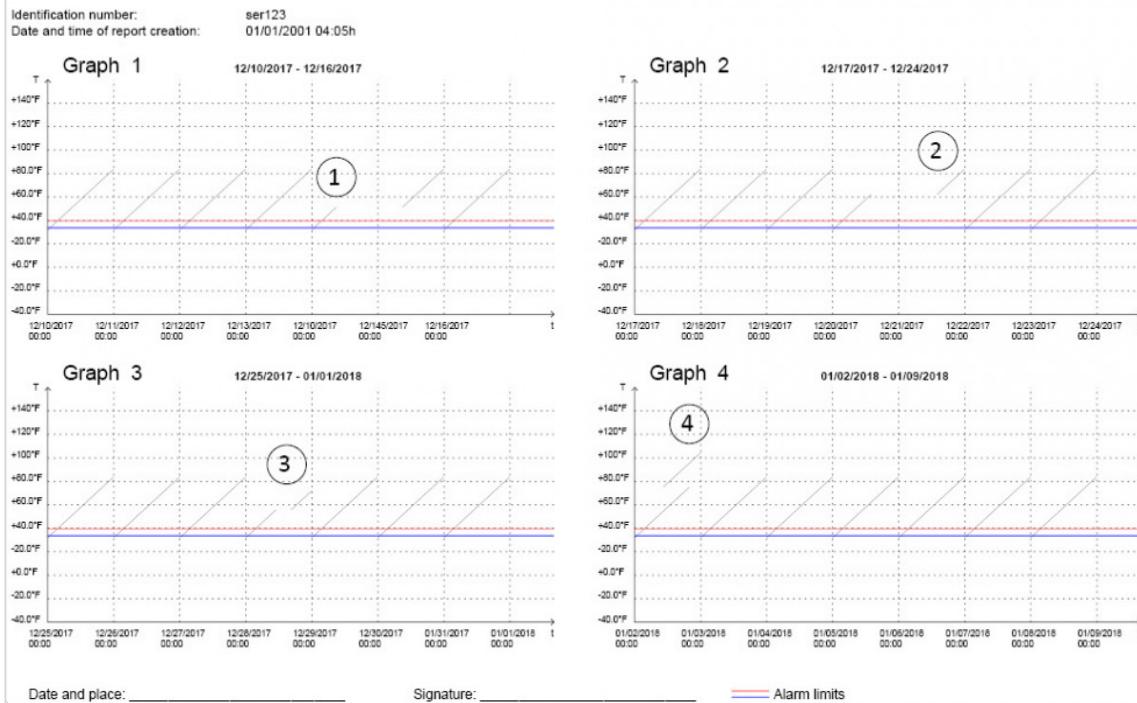

1. Date change positive
2. Date change negative
3. Time change positive (e.g. summer/winter time)
4. Time change negative (e.g. summer/winter time)

Autoscaling of Graphs in PDF

The graph of the report is created dynamically depending on the following settings:

- the alarm limits of the device.
- the highest and lowest measured value.


This is valid for all graphs in the PDF file until:

- highest and lowest values drop out of history.
- temperature settings are changed (self-configurable device only).


Example below: The scale of the graph depends on the alarm limits set. The temperature scale ranges from +40°C to -5°C for the limits of +0.5°C and +28°C.



Example below: The scale of the graph depends on the highest and lowest measured temperature values. The temperature scale ranges from -30°C to +60°C. Lowest measured temperature: -12°C, highest measured temperature: +25°C.

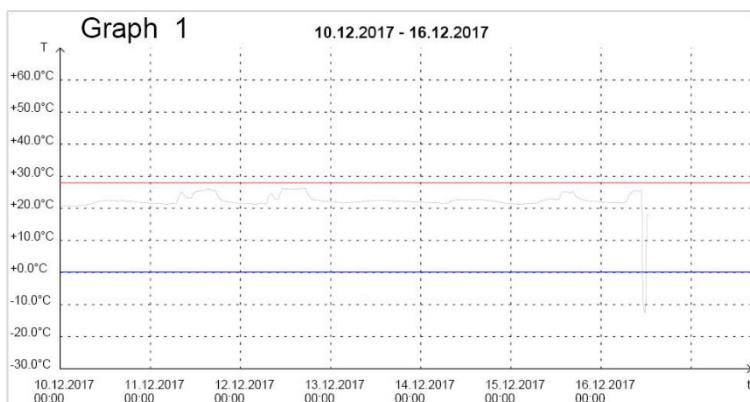

Sample of a PDF file generated by a Fridge-tag with internal sensor:

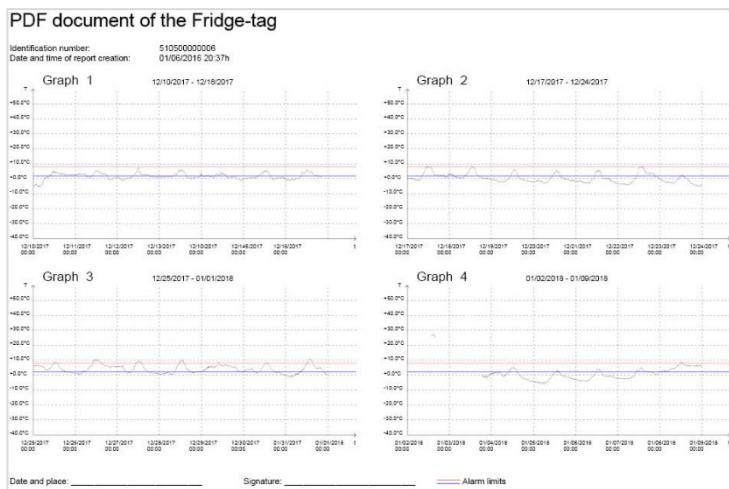

PDF document of the Fridge-tag

Identification number: 510500000006
 Date and time of report creation: 01/06/2016 20:37h
 Activation date: 12/10/2015 13:40h
 Upper alarm limit: Above +8.0°C for 1min
 Lower alarm limit: Below +2.0°C for 1min
 Measurement interval:¹⁾ 1min (fixed)
 Logging interval: 5min

No.	Date (MM/dd/yyyy)	Events ²⁾	Average temp.	Lower alarm limit		Upper alarm limit		Signature / notes Action taken	
				Status	Mn. temp.	Cumulative daily time below the limit	Status		
1	Today 01/05/2016	+1.8°C +1.5°C +1.5°C +1.0°C +1.7°C +2.3°C +0.9°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-1.0°C -0.5°C -1.0°C -0.1°C -1.1°C -0.7°C -5.3°C	11h 4min 15h 2min 16h 1min 16h 8min 14h 54min 9h 35min 9h 24min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	In progress ok ok ok ok ok ok	+8.5°C +4.7°C +4.5°C +6.4°C +7.5°C +5.6°C +5.3°C	0min 0min 0min 0min 0min 0min 0min
2	12/29/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	22h 46min 20h 1min 19h 42min 19h 47min 13h 19min 11h 14min	00:01h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+2.5°C +8.0°C +5.9°C +6.4°C +8.3°C +8.6°C	0min 13:48h 0min 0min 24min 30min
3	12/28/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 26min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
4	12/27/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 25min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
5	12/26/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 24min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
6	12/25/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 23min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
7	12/24/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 22min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
8	12/23/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 21min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
9	12/22/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 20min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
10	12/21/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 19min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
11	12/20/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 18min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
12	12/19/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 17min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
13	12/18/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 16min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
14	12/17/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 15min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
15	12/16/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 14min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
16	12/15/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 13min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
17	12/14/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 12min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
18	12/13/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 11min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
19	12/12/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 10min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
20	12/11/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 9min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
21	12/10/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 8min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
22	12/09/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 7min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
23	12/08/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 6min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
24	12/14/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 5min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
25	12/13/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 4min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
26	12/12/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 3min 19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:00h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 0min 0min 0min 24min 35min
27	12/11/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 2min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:27h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 2h 20min 0min
28	12/10/2015	+0.9°C -0.3°C +0.9°C +0.9°C +2.3°C +2.4°C	ALARM! ALARM! ALARM! ALARM! ALARM! ALARM!	-5.1°C -3.4°C -2.9°C -2.2°C -0.5°C -1.2°C	19h 1min 19h 42min 19h 47min 13h 19min 11h 14min	00:00h 00:26.7h 00:00h 00:00h 00:00h 00:00h	ok ok ok ok ok ok	+8.0°C +5.9°C +6.4°C +6.4°C +8.3°C +8.8°C	0min 13:42h

1) Sampling and data analysis every minute

2) 1 = time/date changed, a = alarm configuration changed, hh:mm = status checked

Date and place: _____ Signature: _____

Date:	Date of measurement
Event: t	Time/date changed
Event: a	Alarm configuration changed
Event: hh:mm	Time stamp: status checked
Average temp.	Average temperature
Status: in progress	The data collection "Today" is not yet complete
Status: OK	No alarm has been triggered in the past 30 days. (No alarm has yet been triggered since the data was read out on the device. *)
Status: Alarm Δ	Alarm(s) have been triggered (With alarm symbol Δ means that the details of the corresponding alarm have not been read out yet. *)
Status: Alarm	Alarm(s) have been triggered (Without alarm symbol $\Delta</math$

Cum. duration	Cumulative daily time below/above the limit
Alarm trigger time	Time at which the alarm was triggered
Max. temp.	Highest recorded temperature
Duration	Duration of an external sensor connection error

*For more information, please refer to the [Alarm Trigger Function](#) section.

Verification process

This process verifies if the files (PDF and ASCII) created by the Fridge-tag are authentic and have not been manipulated or accidentally changed (meets the strict FDA 21 CFR Part 11 requirements).

Note: Please ensure that the latest version of "JAVA Runtime" is previously installed on your computer.

1. Download the software Verifier from our website: <https://sensitech.info/Verifier>.
2. Open the software. The following window will appear:



3. Click **Open file**.
4. Select the file you would like to verify.
 - a) Select the files directly from the Fridge-tag which is connected to your computer.
 - b) Select the files from the place where you saved them on your computer.

When the file is correct and in its original condition, the following window will appear:



In case the file has been changed, an error message will appear.



Proceed the same way with PDF and ASCII files. The same OK or error messages will appear.

Explanations of Terms

Readout mode:

In order to avoid incorrect data, the Fridge-tag does not measure the temperature while settings are changed or during the Readout mode (e.g. changing time, date and during reading of history). The Fridge-tag will fall back into normal operation after approx. 60 seconds without pressing any buttons.

External sensor:

After 10 minutes (factory setting) without connection between external sensor and device, two audio signals sound every three minutes for a maximum of 168 hours (7 days) and the entire display starts flashing.

HI or LO indicator (external sensor):

If the Fridge-tag measures temperatures above +55°C or below -40°C, it shows HI or LO on the screen. The temperature will not be logged and not be shown in the PDF/ASCII file. The regular measurements and monitoring of alarm limits will continue as usual. As soon as the temperature is between +55°C and -40°C numbers will be displayed again.

Expire Code Explanation

Sample: exp 2020-07

The sample shows the expiration date of the Fridge-tag as July 2020 (yyyy-mm).

FAQ / Glossary

Frequently Asked Questions (FAQ)

For technical problems or questions, please refer to sensitech.com page: Fridge-tag 2x Family

Glossary of Symbols

Symbol	Description
✓	OK symbol
✗	alarm symbol
▼	LOW alarm indicator
▲	HIGH alarm indicator
⚠	warning symbol

The warning box includes important information or warnings.